




Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 245

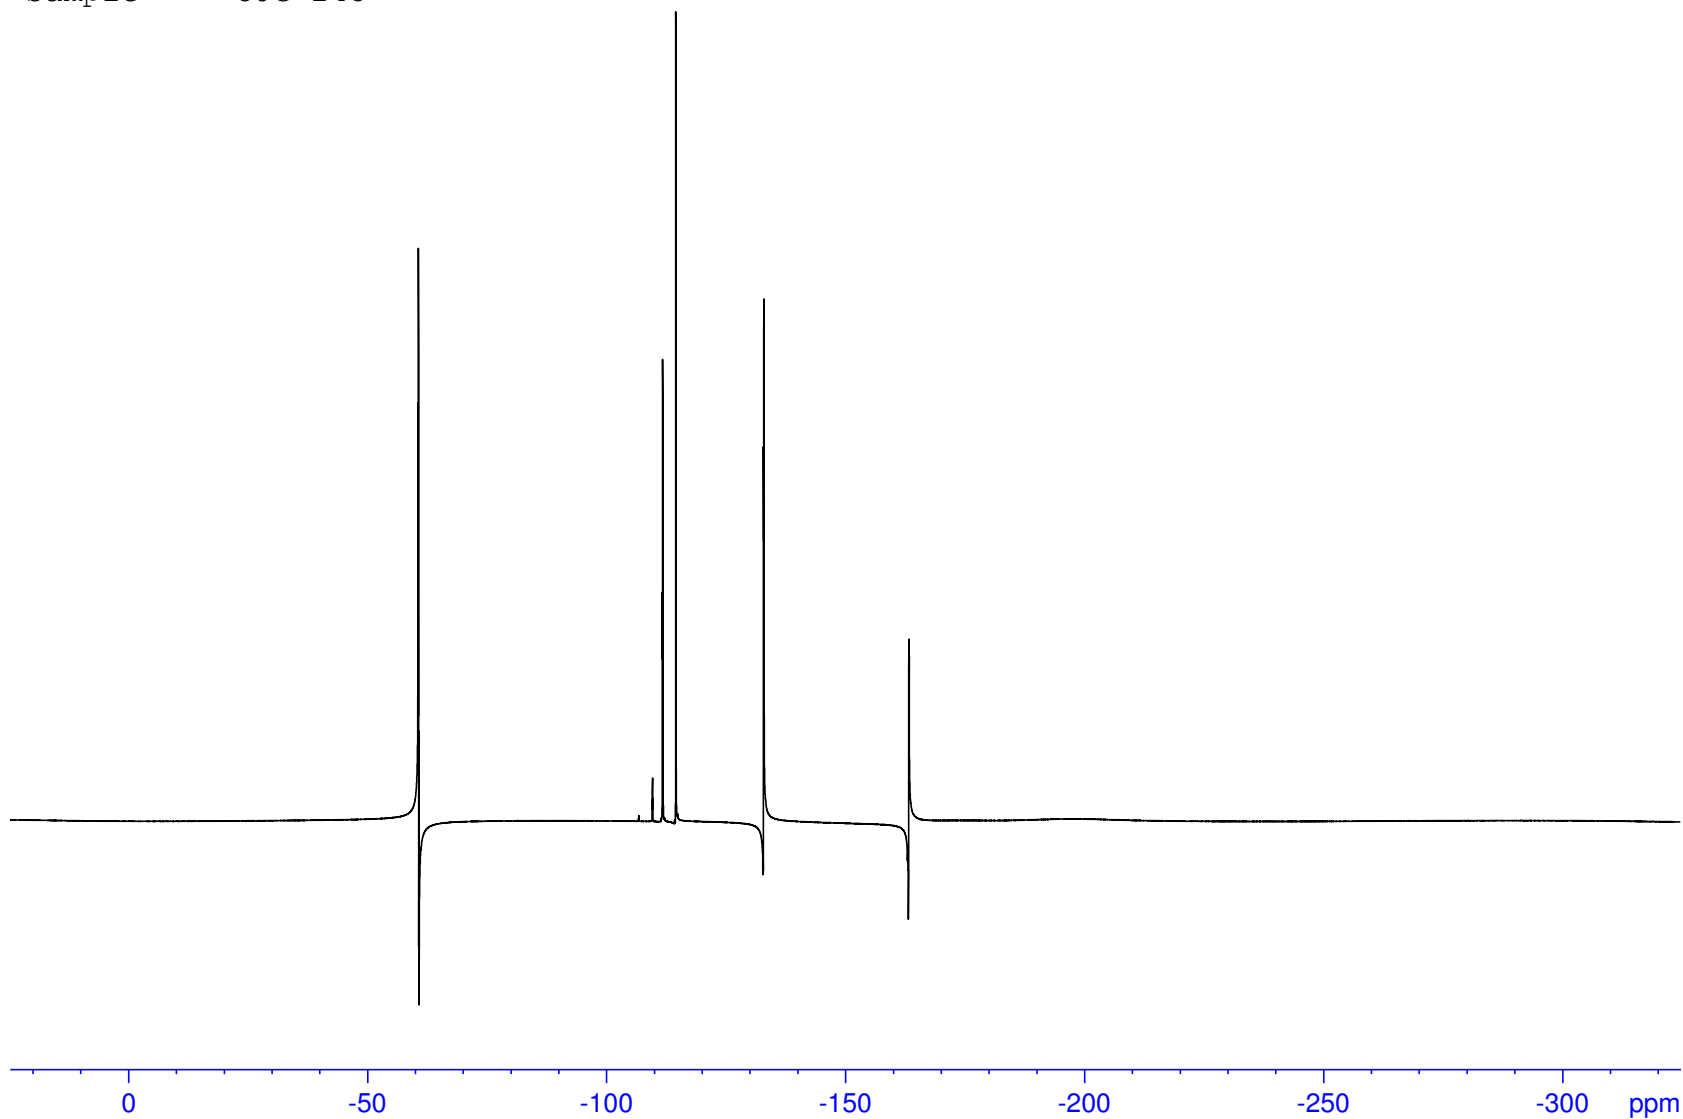

Current Data Parameters
NAME CJG 245 RM 1.33 2
EXPNO 4
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250203
Time 23.45 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 262144
SOLVENT DMSO
NS 32
DS 4
SWH 131578.953 Hz
FIDRES 1.003868 Hz
AQ 0.9961472 sec
RG 201.96
DW 3.800 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 376.4418912 MHz
NUC1 19F
P0 6.00 usec
P1 18.00 usec
PLW1 14.94400024 W

F2 - Processing parameters
SI 65536
SF 376.4983660 MHz
WDW EM
SSB 0
LB 5.00 Hz
GB 0
PC 1.40