

10.91

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 264

Current Data Parameters  
NAME CJG 264 RM 1.33 2  
EXPNO 10  
PROCNO 1


F2 - Acquisition Parameters  
Date\_ 20250204  
Time 0.23 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT DMSO  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.54  
7.51  
7.46  
7.44  
7.43  
7.42  
7.41  
7.39  
7.35  
7.34  
7.33  
7.32  
7.30  
7.30  
6.93  
6.93  
6.91  
6.91  
6.89  
6.89

3.34

2.53  
2.52  
2.51  
2.51  
2.50  
2.50  
2.09

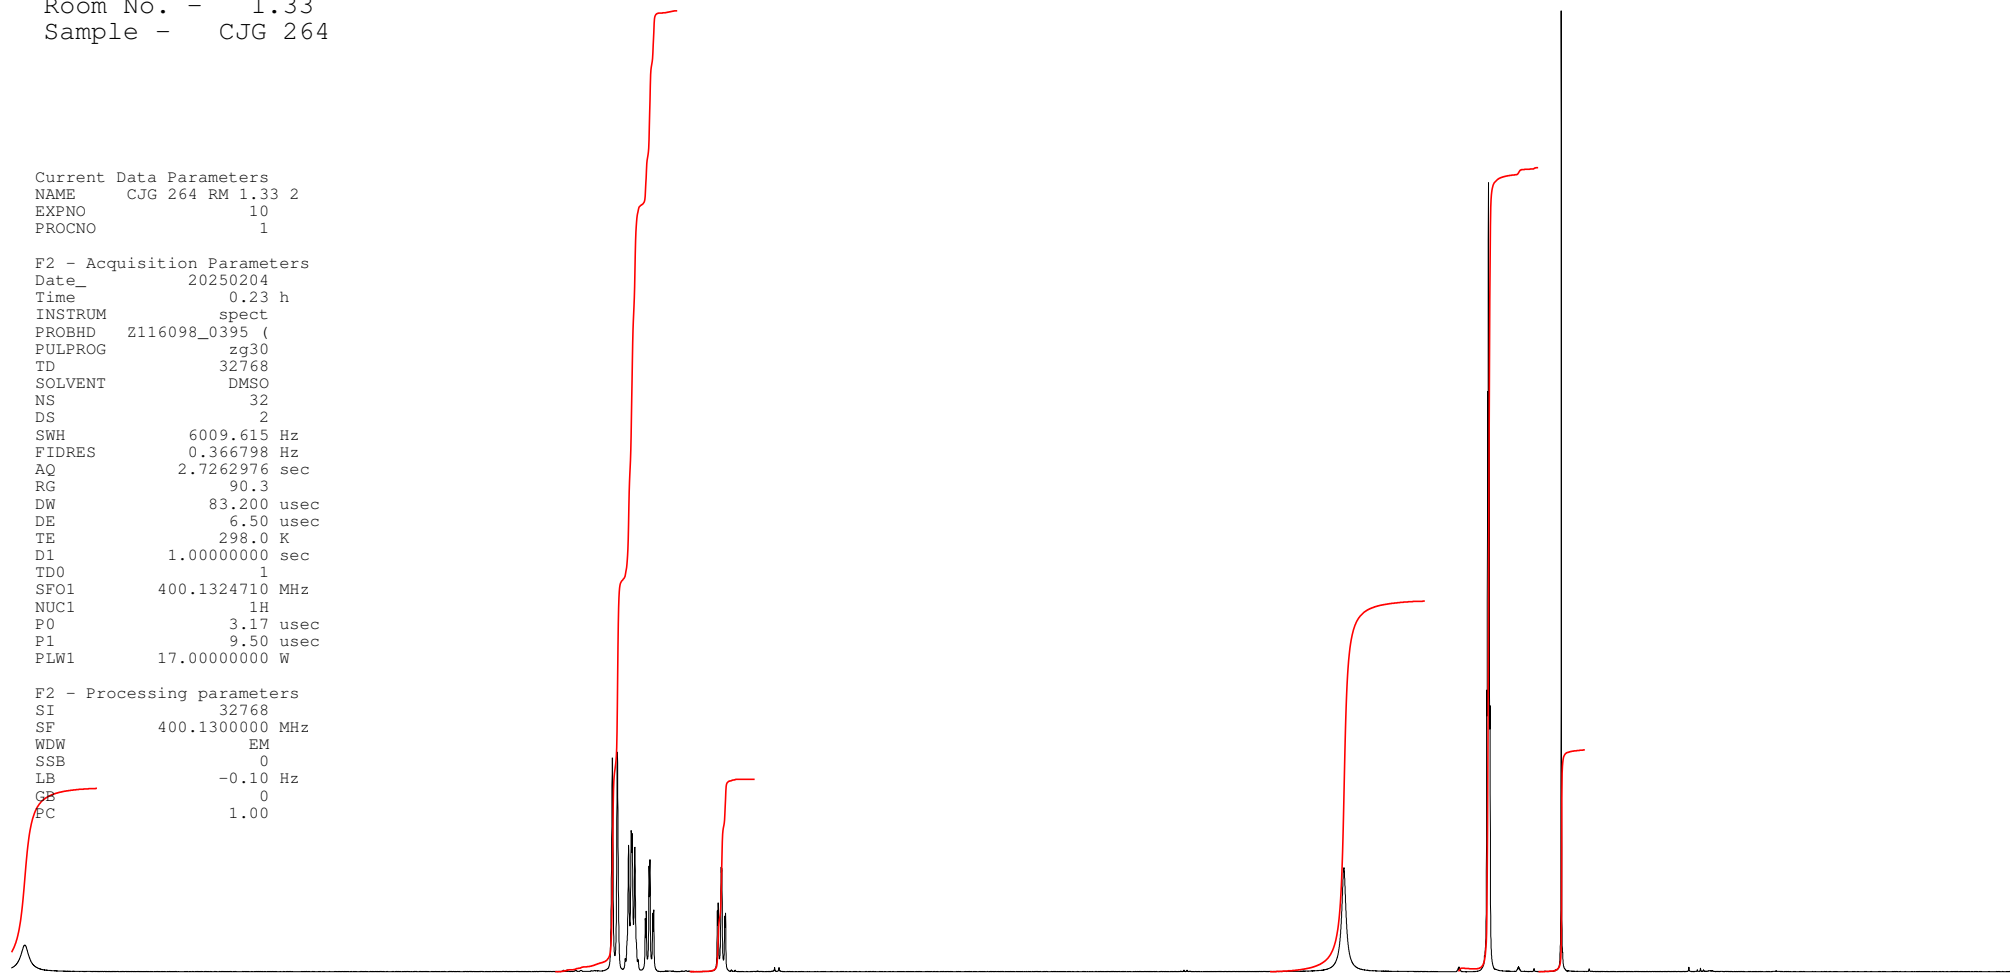

10

9

8

7

6

5

4

3

2

1

0 ppm

35.15

7.04

13.56

29.42

8.12