


Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 253

Current Data Parameters  
NAME CJG 253 (2) RM 1.33  
EXPNO 4  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20241219  
Time 16.04 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300389 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.44  
7.43  
7.42  
7.42  
7.40  
7.19  
7.16  
7.15  
7.14  
7.14  
7.13  
7.13  
7.11  
7.08  
7.07  
6.96  
6.94  
6.93  
6.92  
6.91  
6.89  
— 5.33  
4.21  
4.19  
4.18  
4.16  
3.50  
3.47  
3.44  
2.13  
2.12  
2.11  
2.10  
2.09  
2.08  
2.07  
2.06  
2.05  
2.04  
2.03  
2.03  
2.01  
1.47  
1.33  
1.31  
1.30  
1.29  
1.28  
1.27  
1.25  
1.23  
1.06  
1.04  
1.03  
1.02  
1.00  
0.91  
0.91

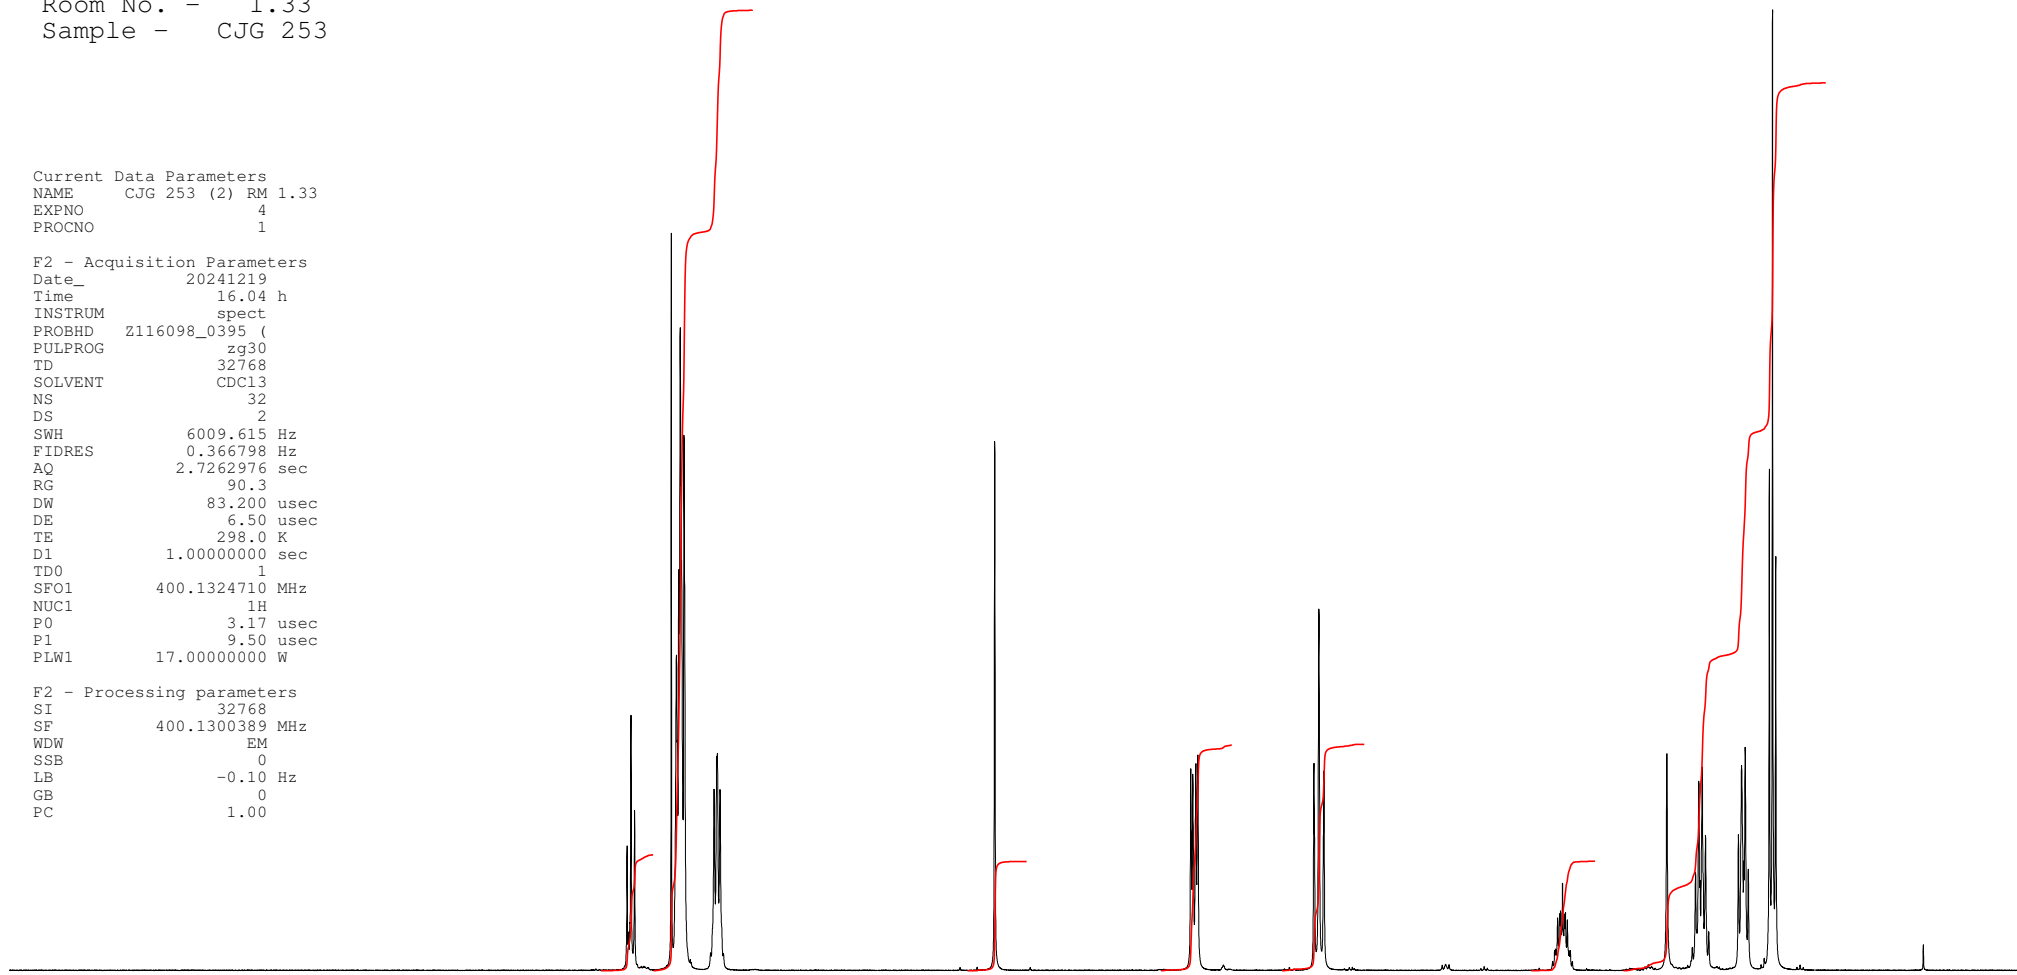

4.40  
36.45

4.15

8.56

8.59

4.16

33.69

0 ppm