




Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 264

124.97
113.81
113.51
113.27
108.51
108.28

40.61
40.41
40.20
39.99
39.78
39.57
39.36
31.14

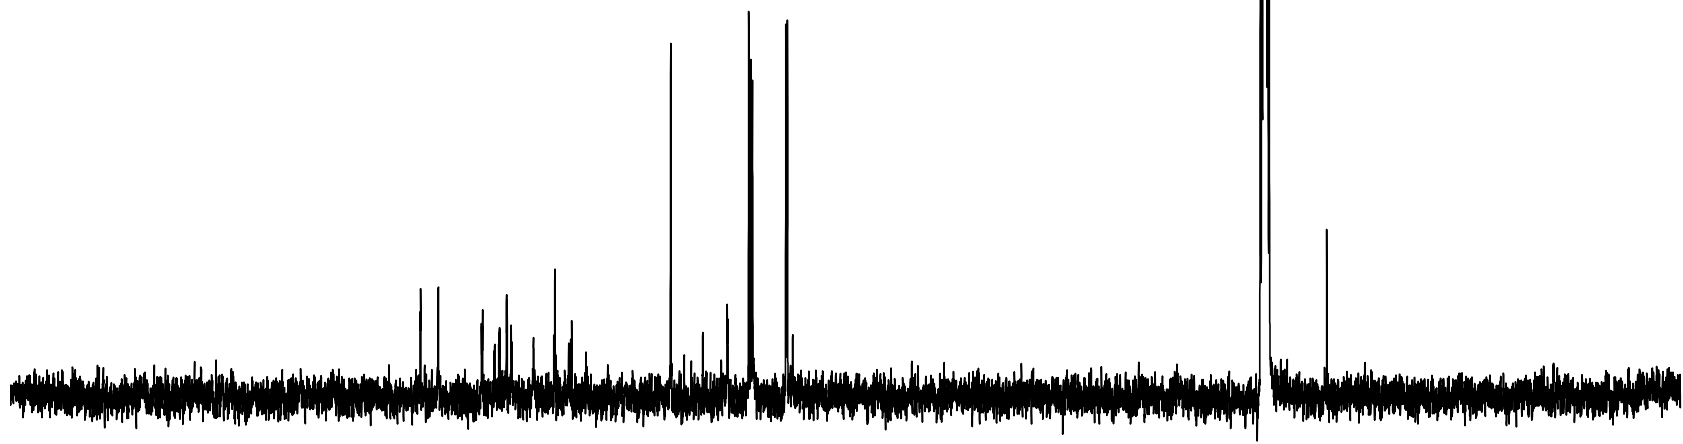

210 200 190 180 170 160 150 140 130 120 110 100 90 80 70 60 50 40 30 20 10 0 ppm

Current Data Parameters
NAME CJG 264 RM 1.33 2
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250204
Time 0.57 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zgpg30
TD 32768
SOLVENT DMSO
NS 1024
DS 8
SWH 24038.461 Hz
FIDRES 1.467191 Hz
AQ 0.6815744 sec
RG 201.96
DW 20.800 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 100.6228298 MHz
NUC1 13C
P0 3.33 usec
P1 10.00 usec
PLW1 60.02999878 W
SFO2 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 17.06500053 W
PLW12 0.21067999 W
PLW13 0.10597000 W

F2 - Processing parameters
SI 65536
SF 100.6127685 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.40