

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 120

Current Data Parameters  
NAME CJG 120 RM 1.33  
EXPNO 1  
PROCNO 1


F2 - Acquisition Parameters  
Date\_ 20231129  
Time 12.27 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300415 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

8.05  
8.02  
7.43  
7.42  
7.41  
7.38  
7.29  
7.27  
7.21  
7.18  
7.12  
7.12  
7.11  
7.11  
7.10  
7.10  
7.09  
7.08

2.72  
2.70  
2.68  
2.66

1.49  
1.24  
1.22  
1.20  
1.18  
1.16  
1.15  
1.15

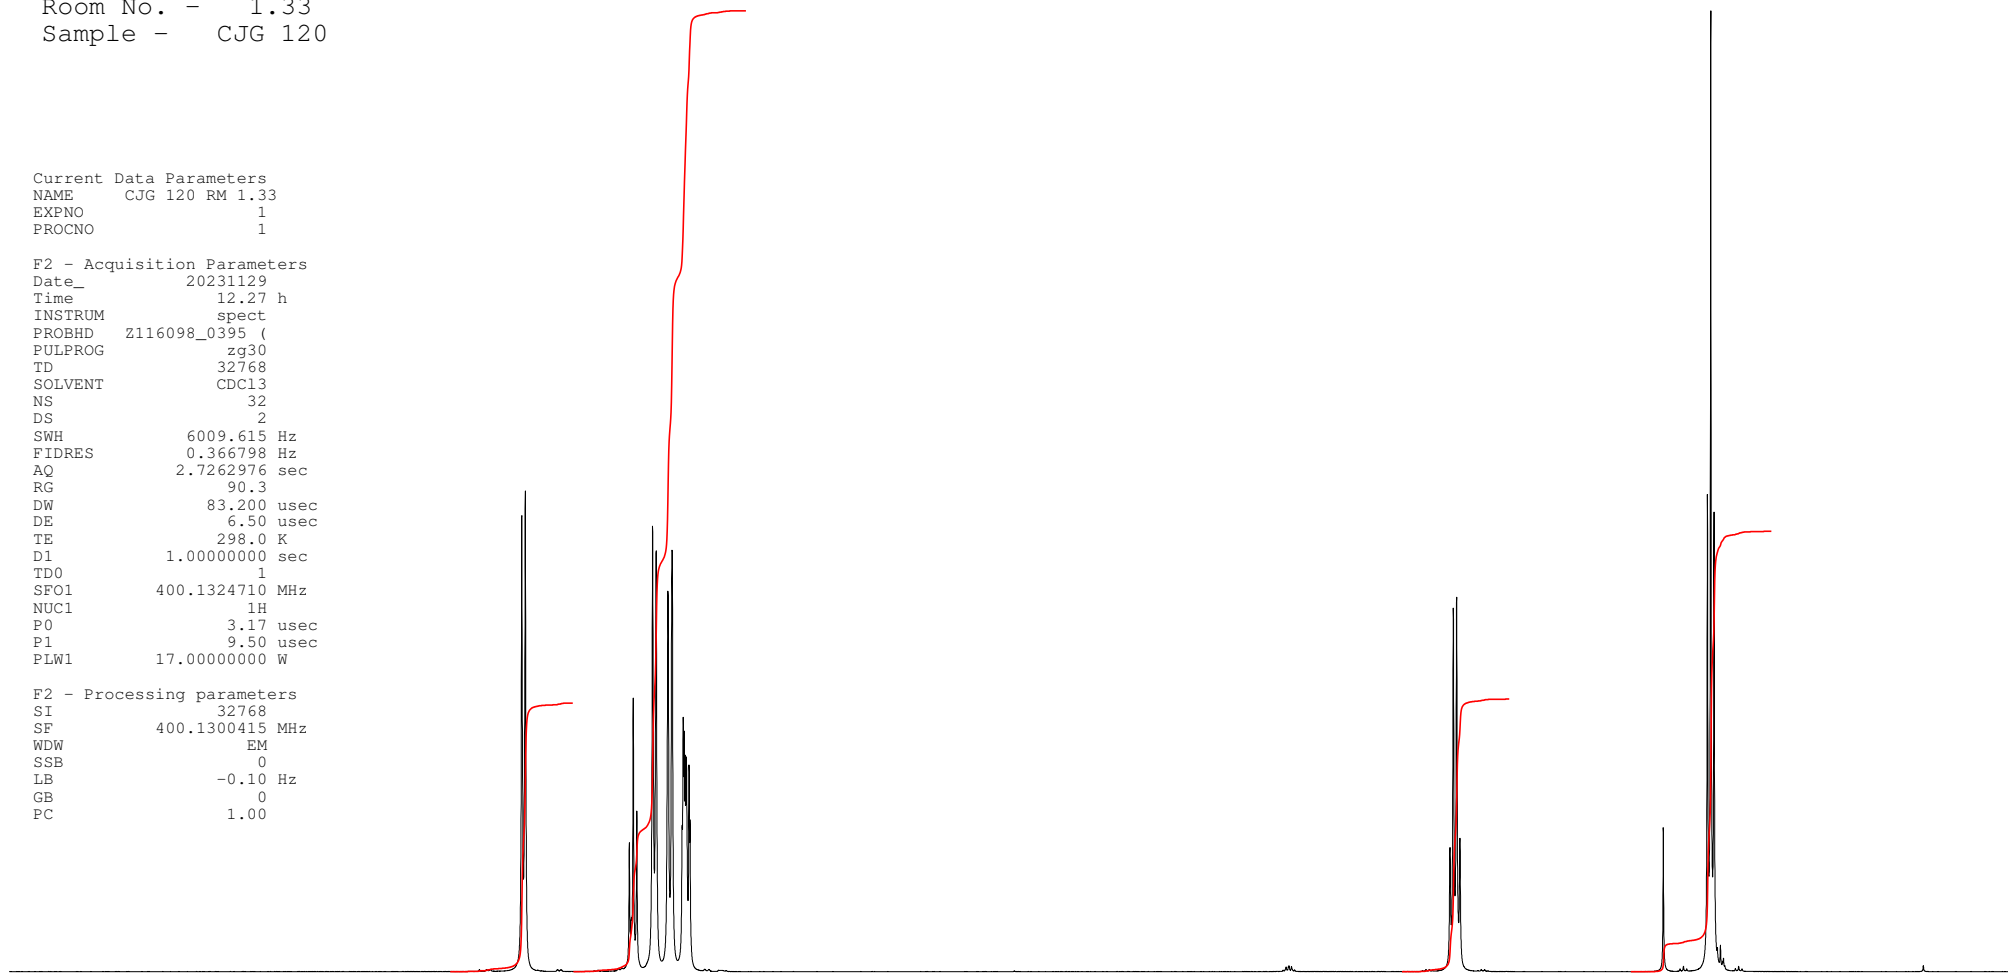

13.83  
49.46

14.04

22.67

0 ppm