

Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 136


Current Data Parameters
NAME CJG 136 (2) RM 1.33
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241118
Time 14.38 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 32768
SOLVENT CDC13
NS 32
DS 2
SWH 6009.615 Hz
FIDRES 0.366798 Hz
AQ 2.7262976 sec
RG 69.08
DW 83.200 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324710 MHz
NUC1 1H
P0 3.17 usec
P1 9.50 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300409 MHz
WDW EM
SSB 0
LB -0.10 Hz
GB 0
PC 1.00

7.95
7.93
7.91
7.64
7.63
7.61
7.43
7.42
7.41
7.39
7.37
7.36
7.34
7.18
7.14
7.14
7.13
7.12
7.12
7.11
7.10
7.09
7.08
7.07
7.04
7.02
6.98
6.95
6.80
6.78

2.62
2.59
2.58
2.57
2.55
1.65
1.65
1.63
1.62
1.60
1.58
1.56
1.50
1.18
1.16
1.14
0.93
0.91
0.90
0.88
-0.00

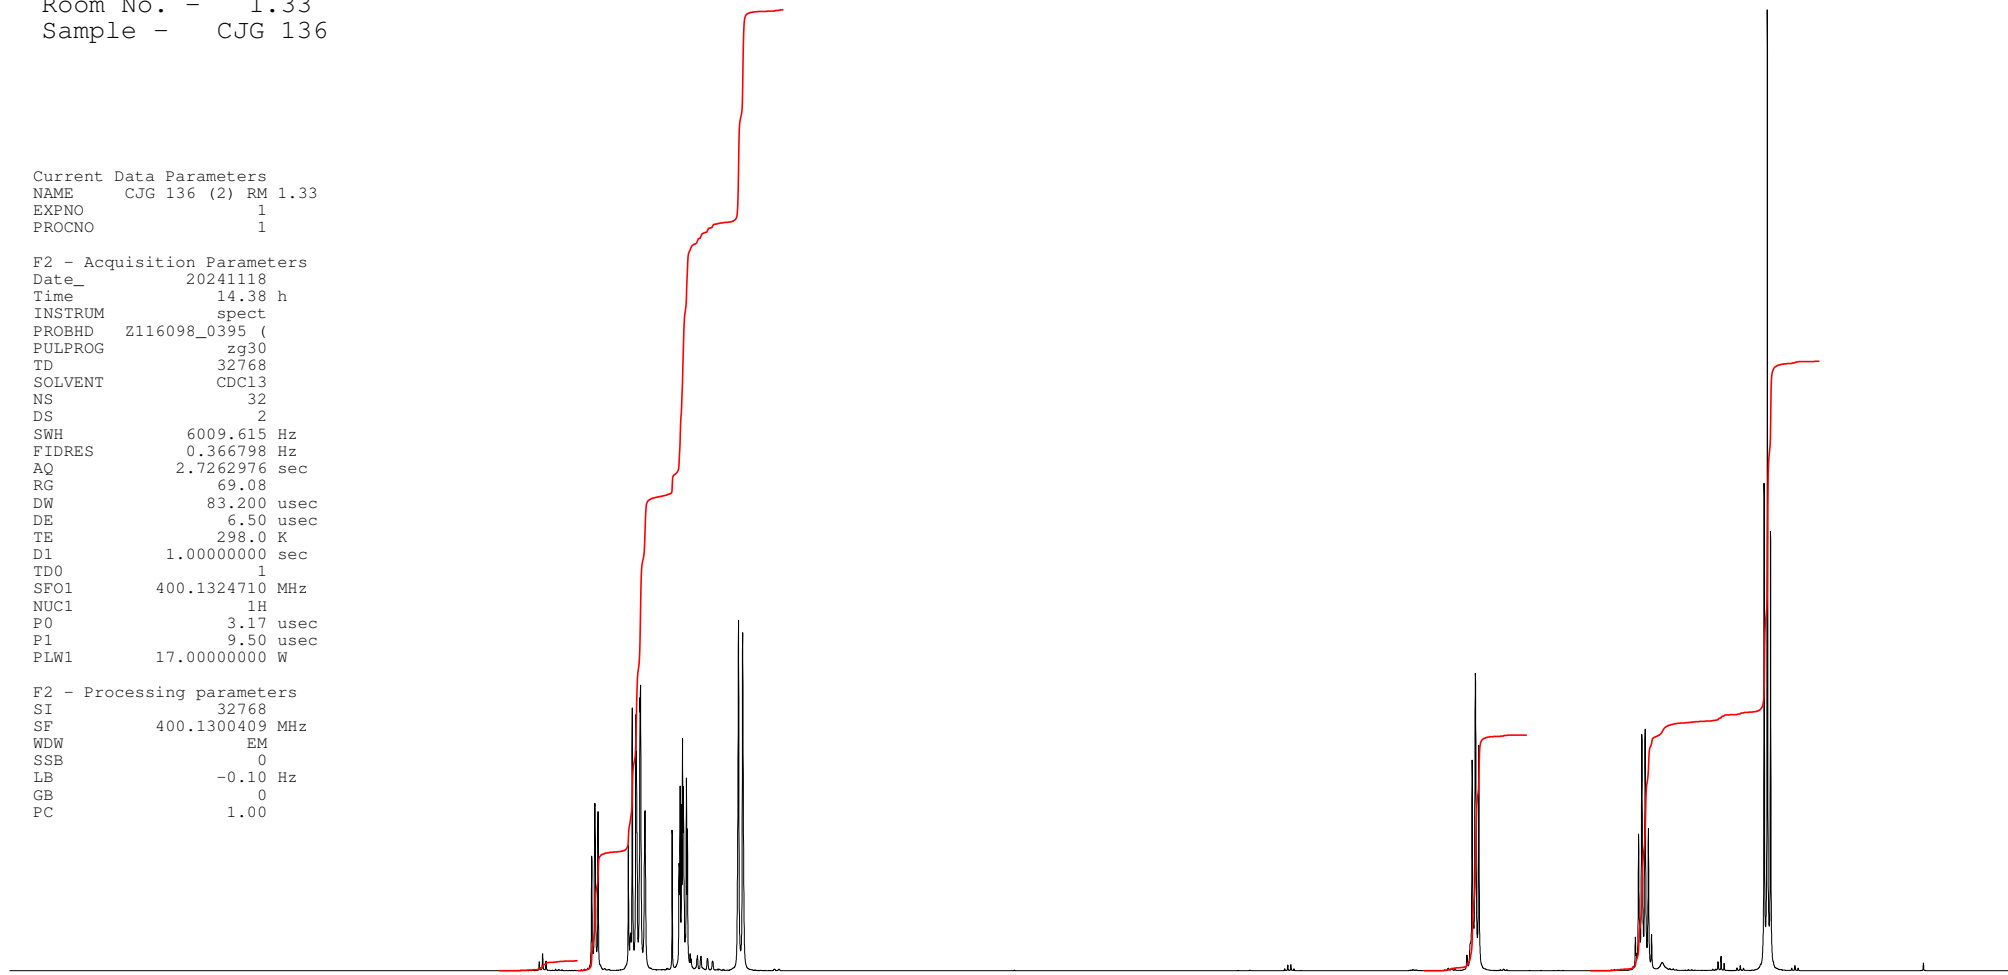

0.55
52.92

12.98
33.56