

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 105

Current Data Parameters  
NAME CJG 105 (2) RM 1.33  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20241011  
Time 12.15 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W


F2 - Processing parameters  
SI 32768  
SF 400.1300398 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.95  
7.93  
7.91  
7.43  
7.42  
7.41  
7.39  
7.20  
7.18  
7.16  
7.15  
7.14  
7.14  
7.12  
7.12  
7.10  
7.04  
7.02  
6.99  
6.96  
6.81  
6.78

2.63  
2.60  
2.58  
2.56

1.66  
1.64  
1.62  
1.60  
1.58  
1.57  
1.49  
0.92  
0.90  
0.88

— 0.00

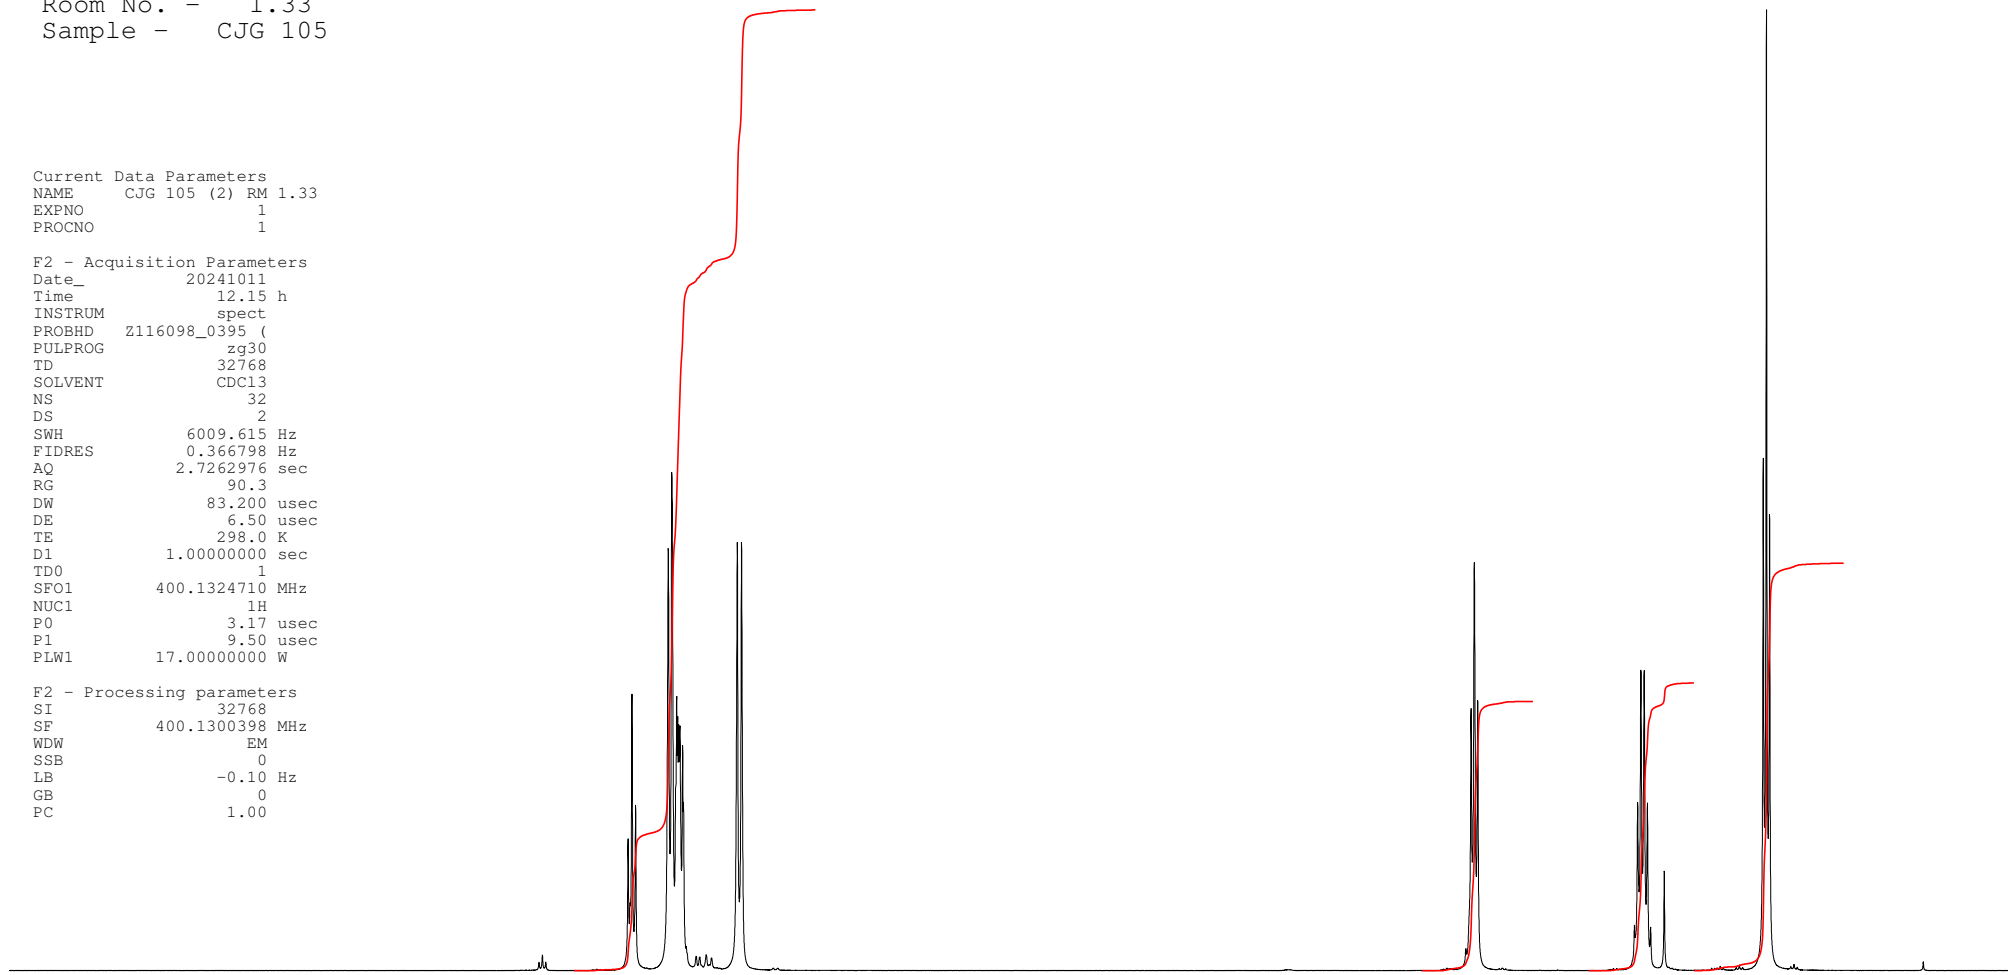

10

9

8

7

6

5

4

3

2

1

0 ppm

49.90

13.99

14.95

21.17