

Name - Calum J Gibb
 Room No. - 1.33
 Sample - CJG 111

Current Data Parameters
 NAME CJG 111 RM 1.33
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20231121
 Time 20.57 h
 INSTRUM spect
 PROBHD Z116098_0395 (
 PULPROG zg30
 TD 32768
 SOLVENT CDC13
 NS 32
 DS 2
 SWH 6009.615 Hz
 FIDRES 0.366798 Hz
 AQ 2.7262976 sec
 RG 90.3
 DW 83.200 usec
 DE 6.50 usec
 TE 298.0 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1324710 MHz
 NUC1 1H
 P0 3.17 usec
 P1 9.50 usec
 PLW1 17.00000000 W


F2 - Processing parameters
 SI 32768
 SF 400.1300393 MHz
 WDW EM
 SSB 0
 LB -0.10 Hz
 GB 0
 PC 1.00

7.96
7.94
7.92
7.68
7.67
7.66
7.63
7.60
7.58
7.45
7.43
7.42
7.41
7.39
7.37
7.19
7.11
7.11
7.10
7.09
7.07
7.06
7.04
7.04
7.02
7.02
7.01
6.99
6.96

3.87
3.83

2.62
2.61
2.59
2.10
1.67
1.65
1.63
1.61
1.60
1.58
1.49
1.19
1.17
1.15
0.92
0.90
0.88

-0.00

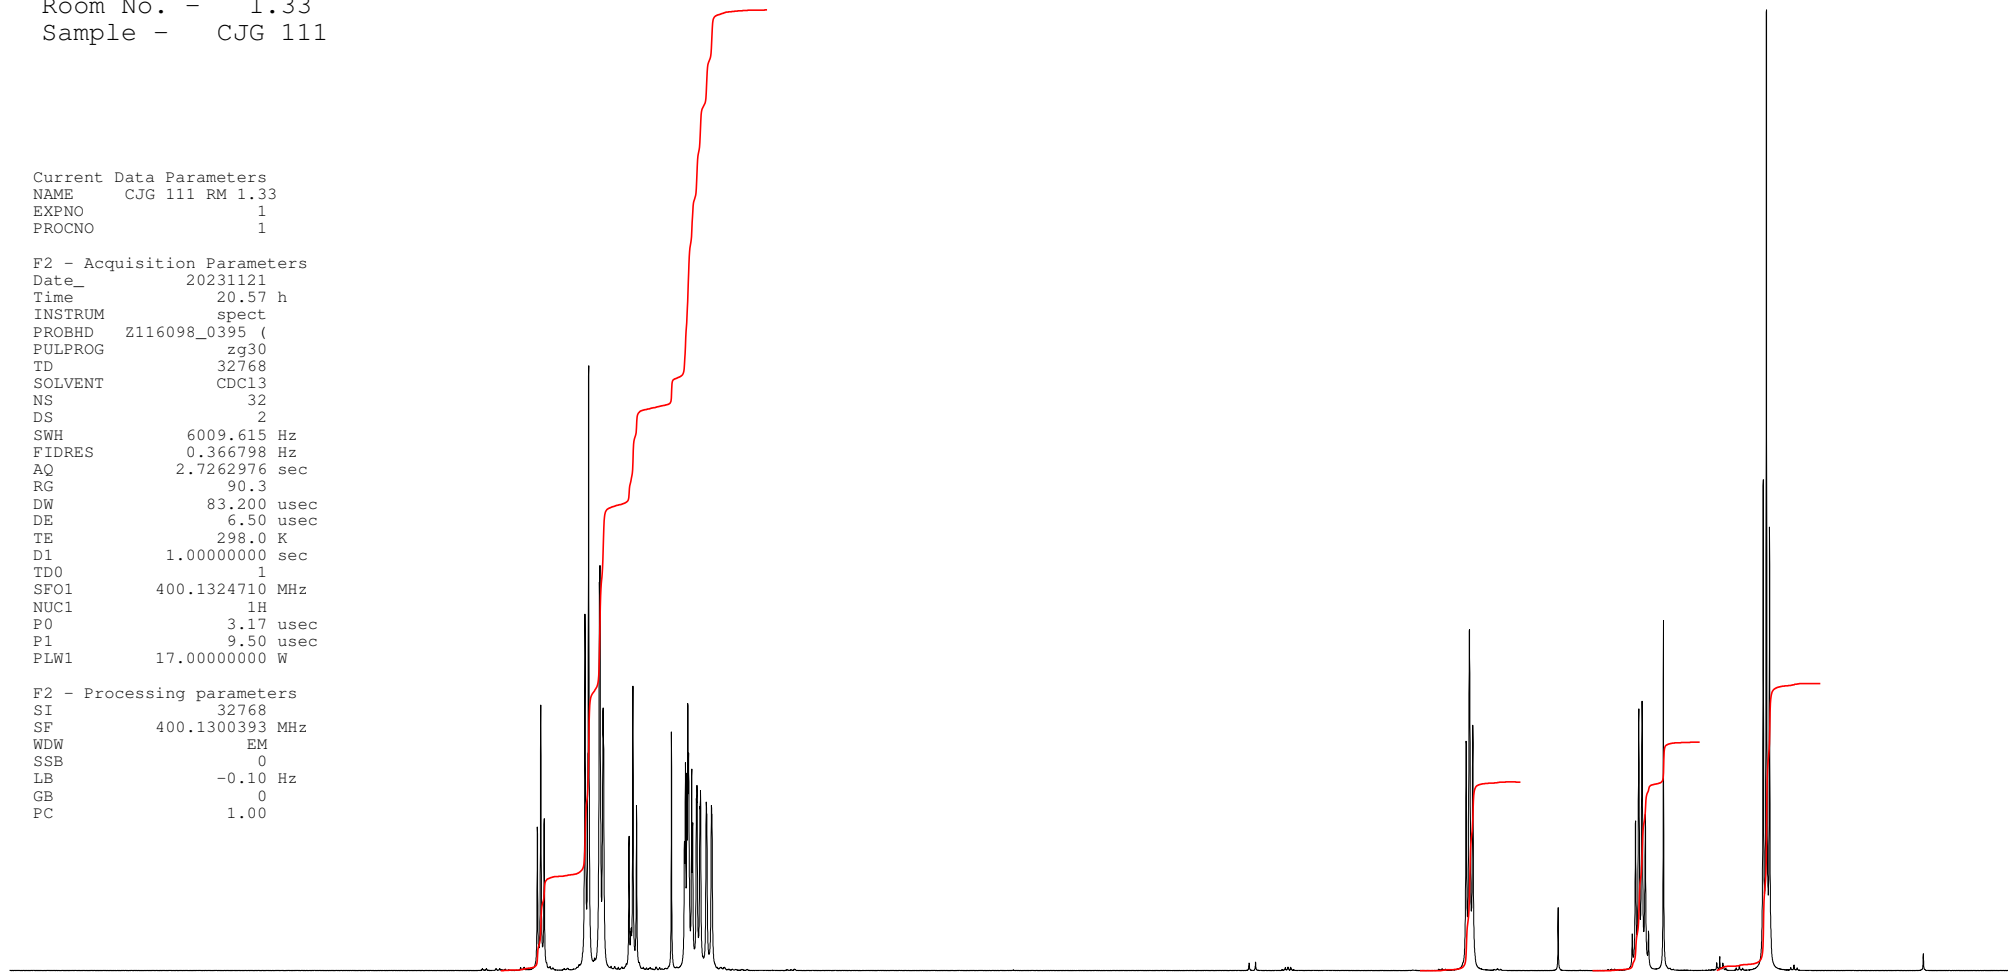

10

9

8

7

6

5

4

3

2

1

0

ppm

57.70

11.33

13.72

17.25