

Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 106


Current Data Parameters
NAME CJG 106
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231120
Time 12.18 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 32768
SOLVENT CDCl3
NS 32
DS 2
SWH 6009.615 Hz
FIDRES 0.366798 Hz
AQ 2.7262976 sec
RG 90.3
DW 83.200 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324710 MHz
NUC1 1H
P0 3.17 usec
P1 9.50 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300385 MHz
WDW EM
SSB 0
LB -0.10 Hz
GB 0
PC 1.00

7.92
7.67
7.65
7.65
7.63
7.34
7.33
7.31
7.29
7.29
7.19
7.00
6.99
6.98
6.96
6.95
6.94
6.94
6.81
6.79

2.63
2.60
2.58
2.56
1.66
1.65
1.64
1.62
1.60
1.59
1.57
1.48
1.19
1.17
1.15
0.92
0.90
0.89
-0.00

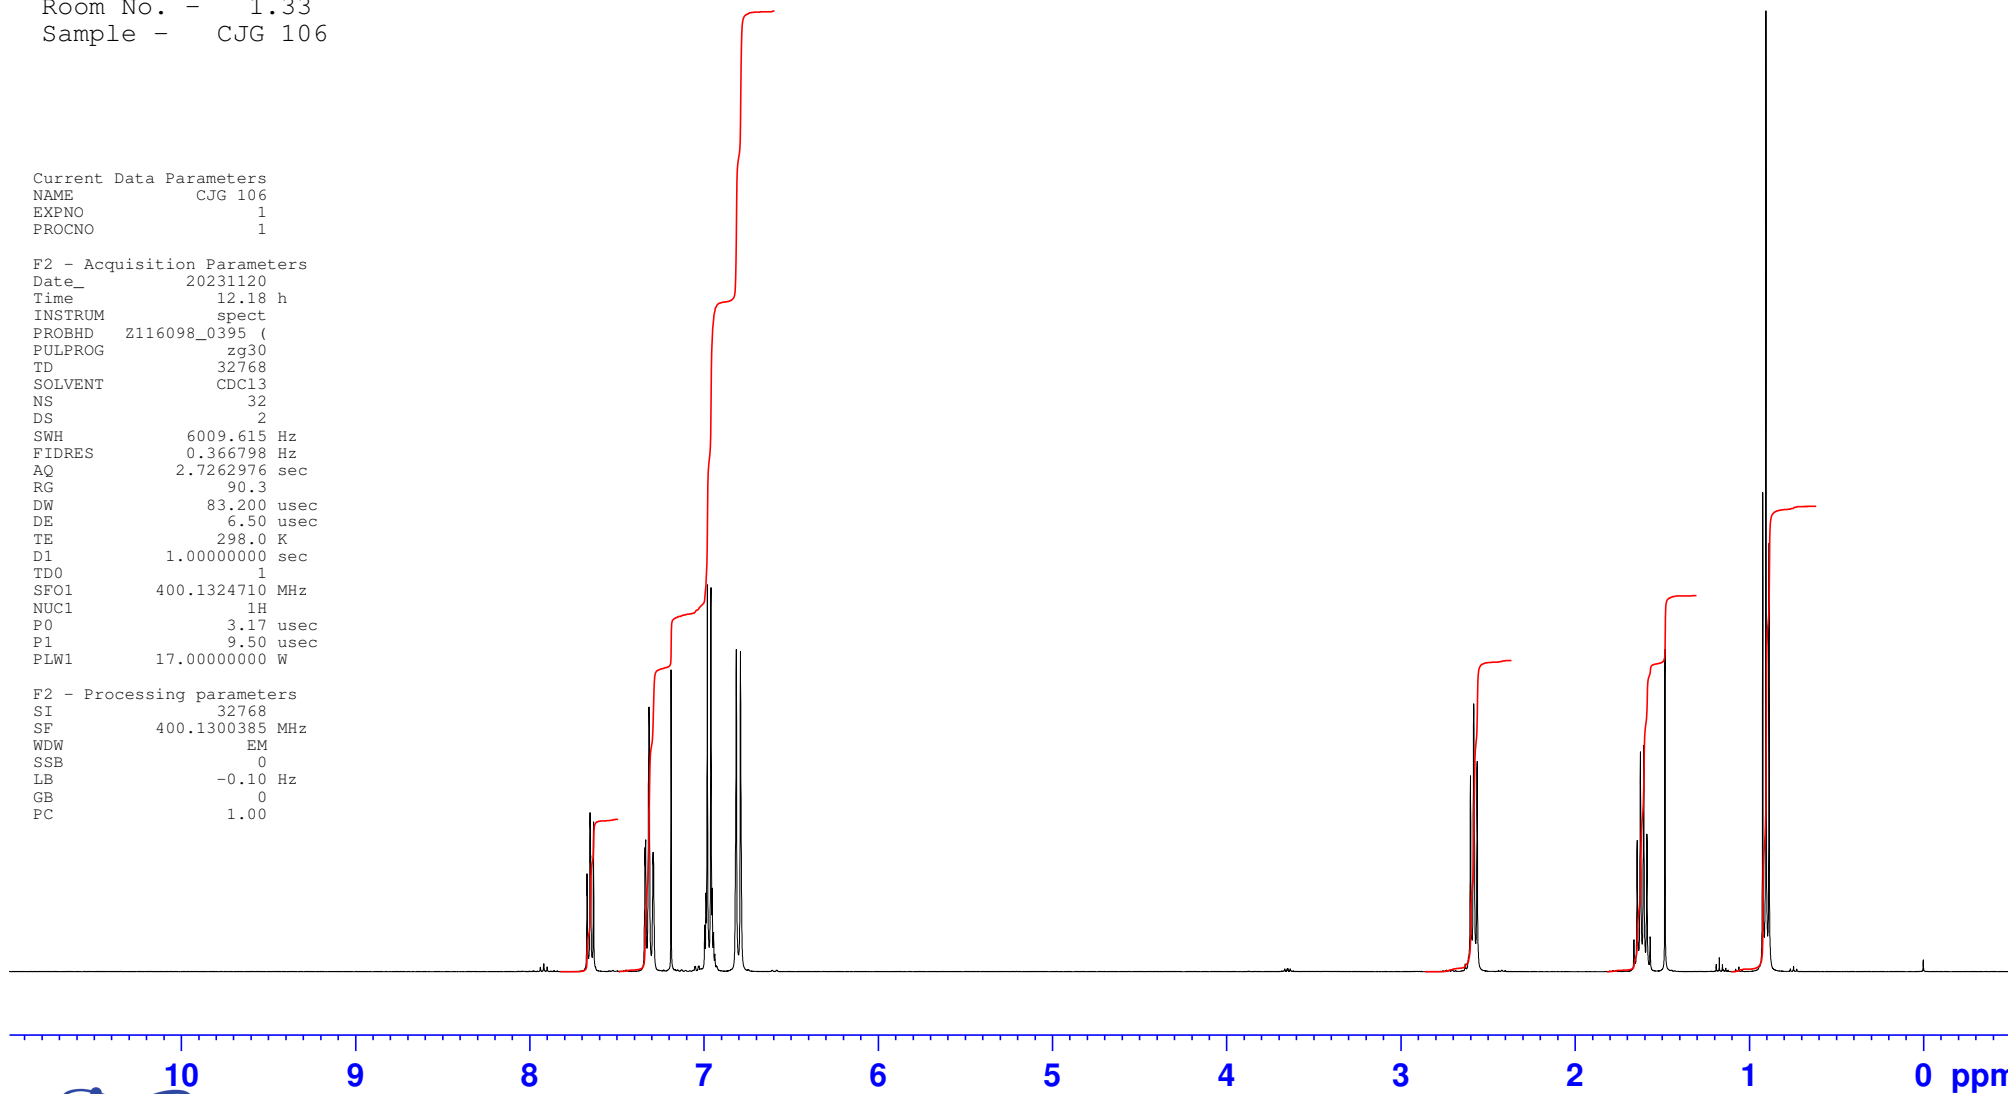

6.73
42.41

13.73

16.59

20.54