

Name - Calum J Gibb
 Room No. - 1.33
 Sample - CJG 101

Current Data Parameters
 NAME CJG 101 RM 1.33
 EXPNO 1
 PROCNO 1


F2 - Acquisition Parameters
 Date_ 20231030
 Time 14.37 h
 INSTRUM spect
 PROBHD Z116098_0395 (
 PULPROG zg30
 TD 32768
 SOLVENT CDC13
 NS 32
 DS 2
 SWH 6009.615 Hz
 FIDRES 0.366798 Hz
 AQ 2.7262976 sec
 RG 90.3
 DW 83.200 usec
 DE 6.50 usec
 TE 298.0 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1324710 MHz
 NUC1 1H
 P0 3.17 usec
 P1 9.50 usec
 PLW1 17.00000000 W

F2 - Processing parameters
 SI 32768
 SF 400.1300381 MHz
 WDW EM
 SSB 0
 LB -0.10 Hz
 GB 0
 PC 1.00

8.07
8.05
7.68
7.67
7.66
7.66
7.63
7.62
7.61
7.61
7.59
7.59
7.58
7.58
7.56
7.56
7.55
7.27
7.25
7.19

3.67
3.66
3.64
3.62

2.64
2.63
2.61
1.68
1.66
1.64
1.62
1.60
1.58
1.55
1.32
1.31
1.22
1.19
1.17
1.15
0.92
0.90
0.88
-0.00

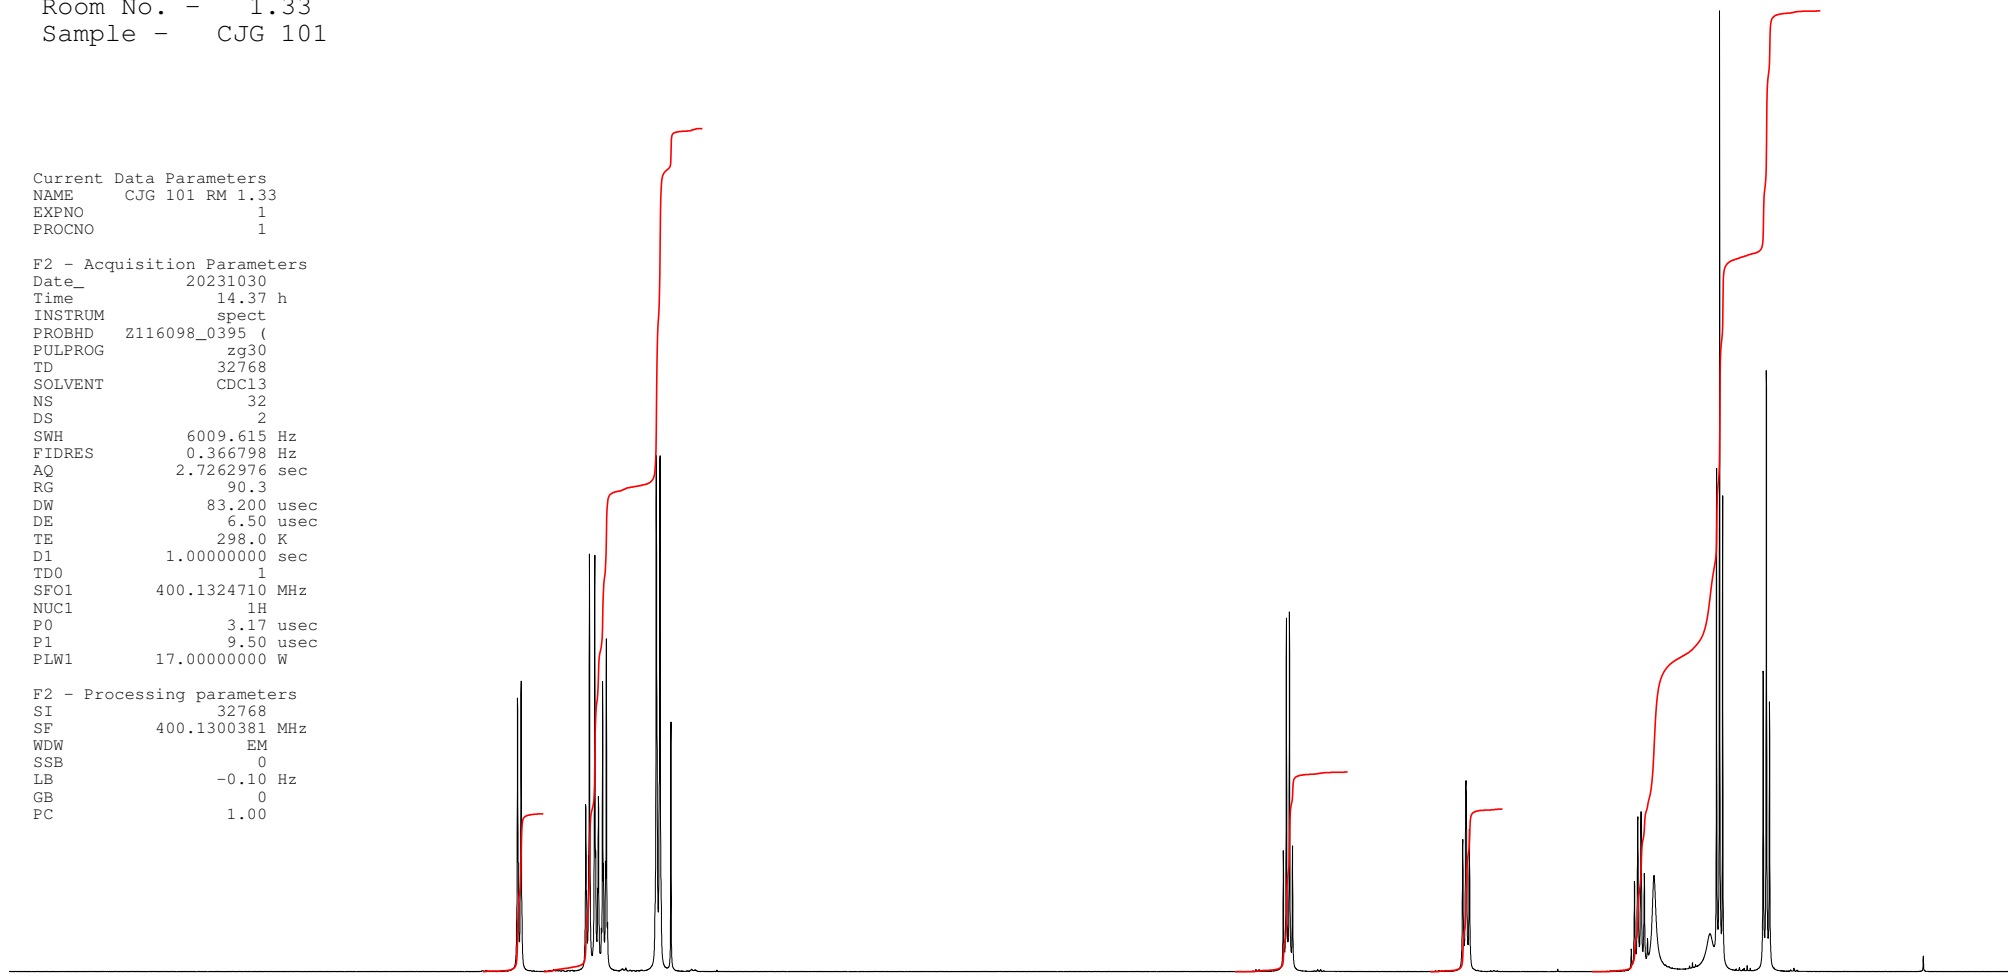

6.79
36.28

8.59

7.00

41.34

0 ppm