

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 104

Current Data Parameters  
NAME CJG 104 RM 1.33  
EXPNO 1  
PROCNO 1


F2 - Acquisition Parameters  
Date\_ 20231106  
Time 11.42 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300382 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.94  
7.92  
7.90  
7.19  
7.15  
7.13  
7.05  
7.03  
7.01  
7.00  
7.00  
6.98  
6.97  
6.96  
6.95  
6.82  
6.79

2.63  
2.60  
2.59  
2.58  
2.56  
1.66  
1.66  
1.64  
1.63  
1.61  
1.59  
1.57  
1.48  
1.17  
0.92  
0.91  
0.89

— -0.00

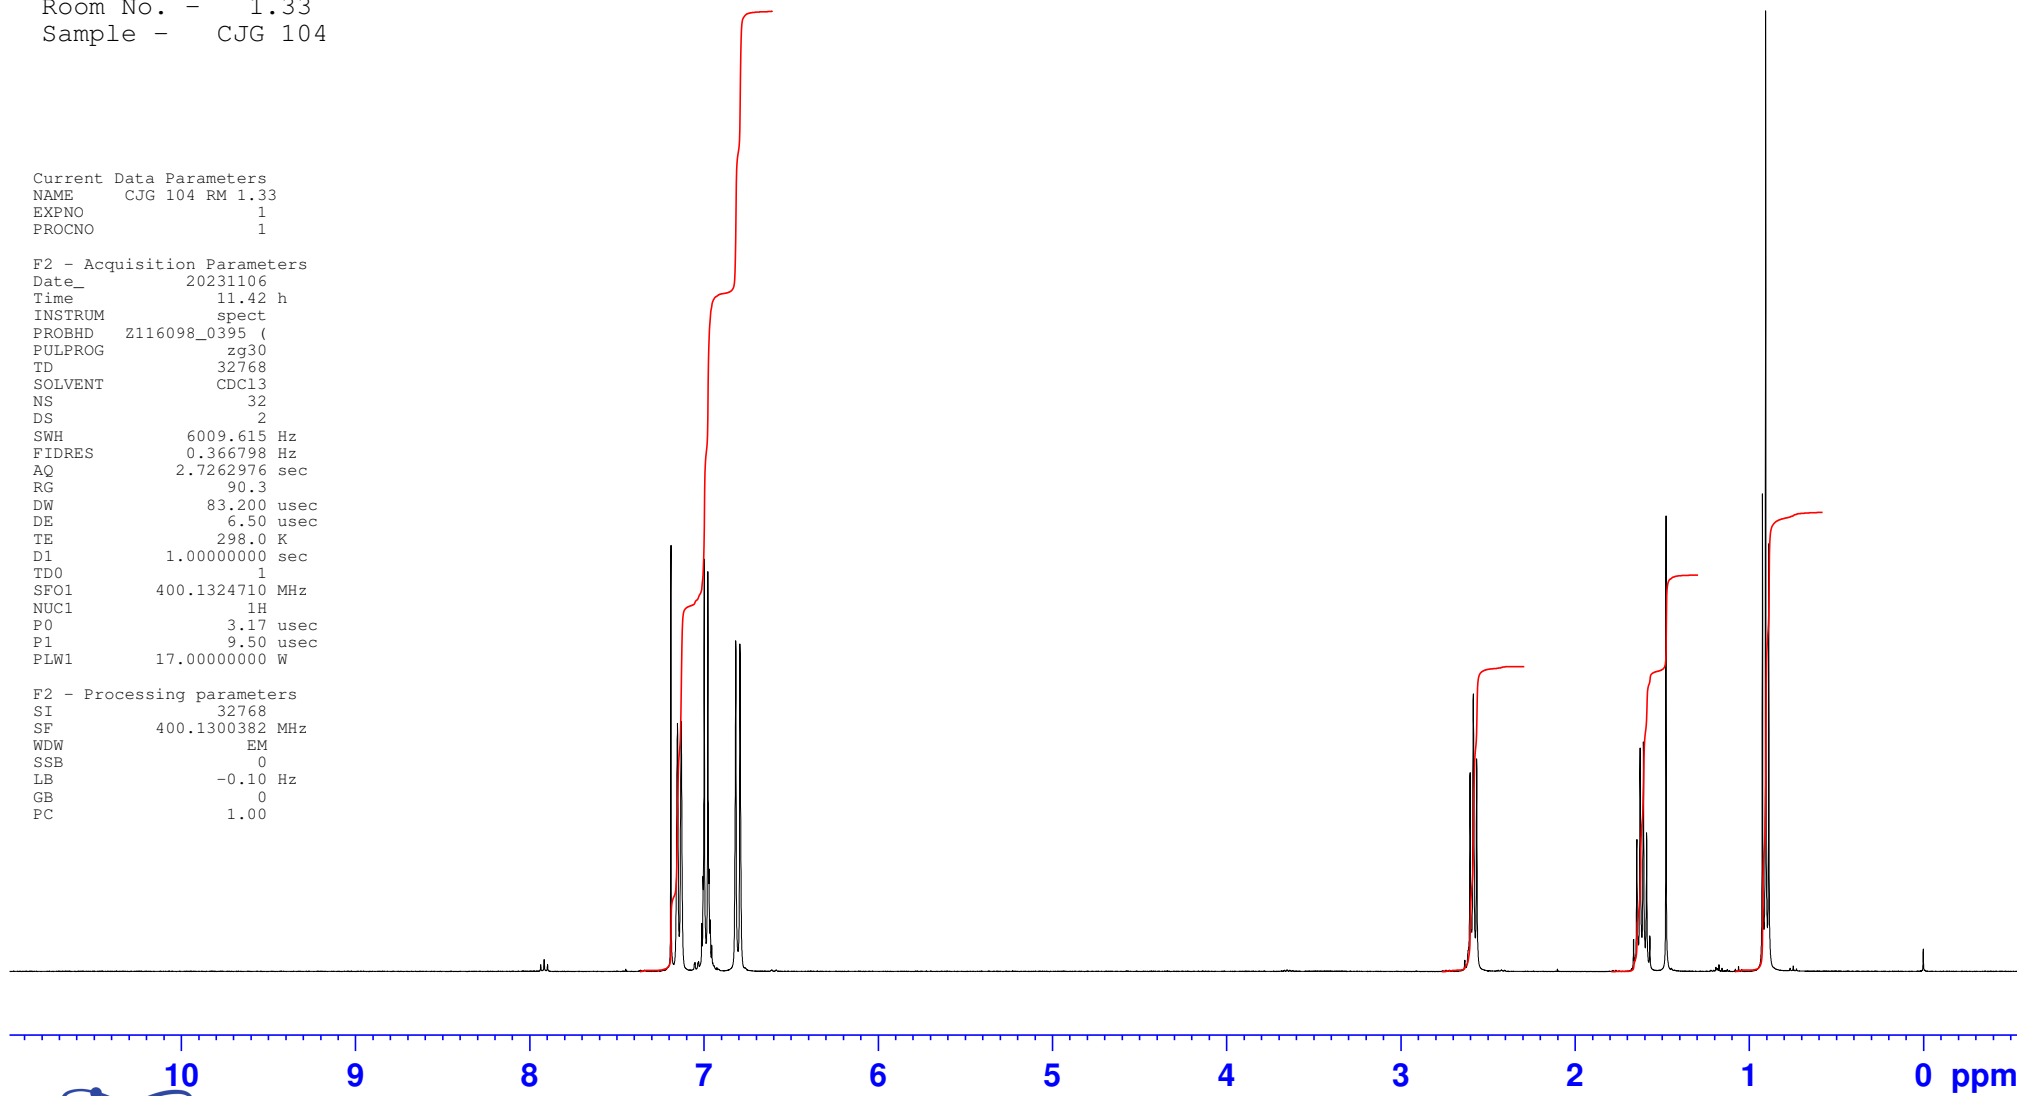

45.28

14.38

18.69

21.65