

Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 96


Current Data Parameters
NAME CJG 96 RM 1.33
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231027
Time 17.12 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 32768
SOLVENT CDC13
NS 32
DS 2
SWH 6009.615 Hz
FIDRES 0.366798 Hz
AQ 2.7262976 sec
RG 90.3
DW 83.200 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324710 MHz
NUC1 1H
P0 3.17 usec
P1 9.50 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300390 MHz
WDW EM
SSB 0
LB -0.10 Hz
GB 0
PC 1.00

8.05
8.03
8.00
7.98
7.47
7.43
7.41
7.39
7.28
7.26
7.21
7.19
7.12
7.11
7.10
7.09

2.70
2.65
2.63
2.61
2.10
1.68
1.66
1.64
1.62
1.60
1.58
1.48
1.19
1.17
1.15
1.06
0.92
0.88
-0.00

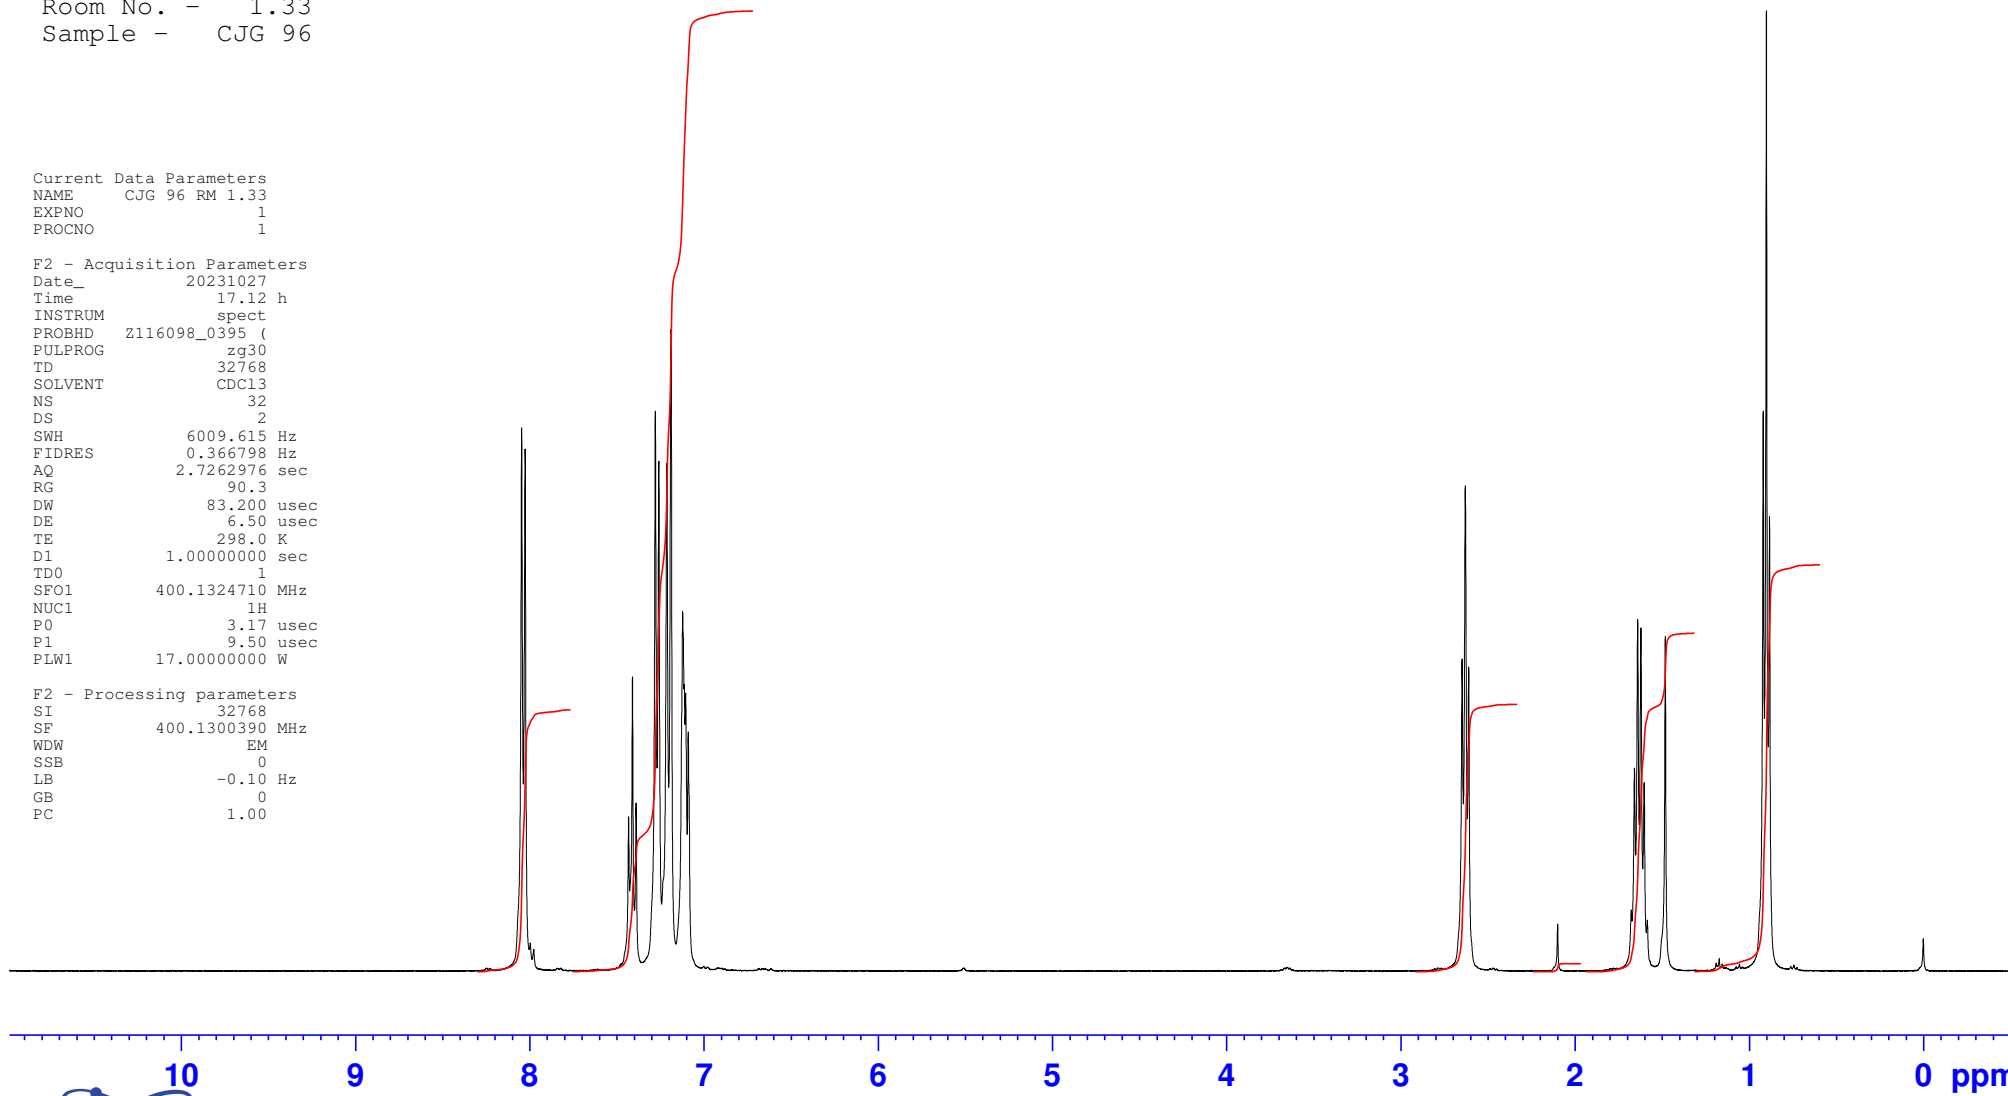

11.67
42.83

11.91
0.36
15.09
18.14