

Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 98

Current Data Parameters
NAME CJG 98 RM 1.33
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231030
Time 14.27 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 32768
SOLVENT CDC13
NS 32
DS 2
SWH 6009.615 Hz
FIDRES 0.366798 Hz
AQ 2.7262976 sec
RG 90.3
DW 83.200 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324710 MHz
NUC1 1H
P0 3.17 usec
P1 9.50 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300381 MHz
WDW EM
SSB 0
LB -0.10 Hz
GB 0
PC 1.00


8.04
8.03
8.03
8.02
8.01
8.01
7.28
7.26
7.19
7.16
7.14
6.97
6.97
6.96
6.94
6.93
6.92

3.67
3.66
3.65
3.64

2.65
2.63
2.61

1.68
1.66
1.64
1.62
1.60
1.59
1.47
1.19
1.17
1.16
1.12
0.92
0.90
0.88

-0.00

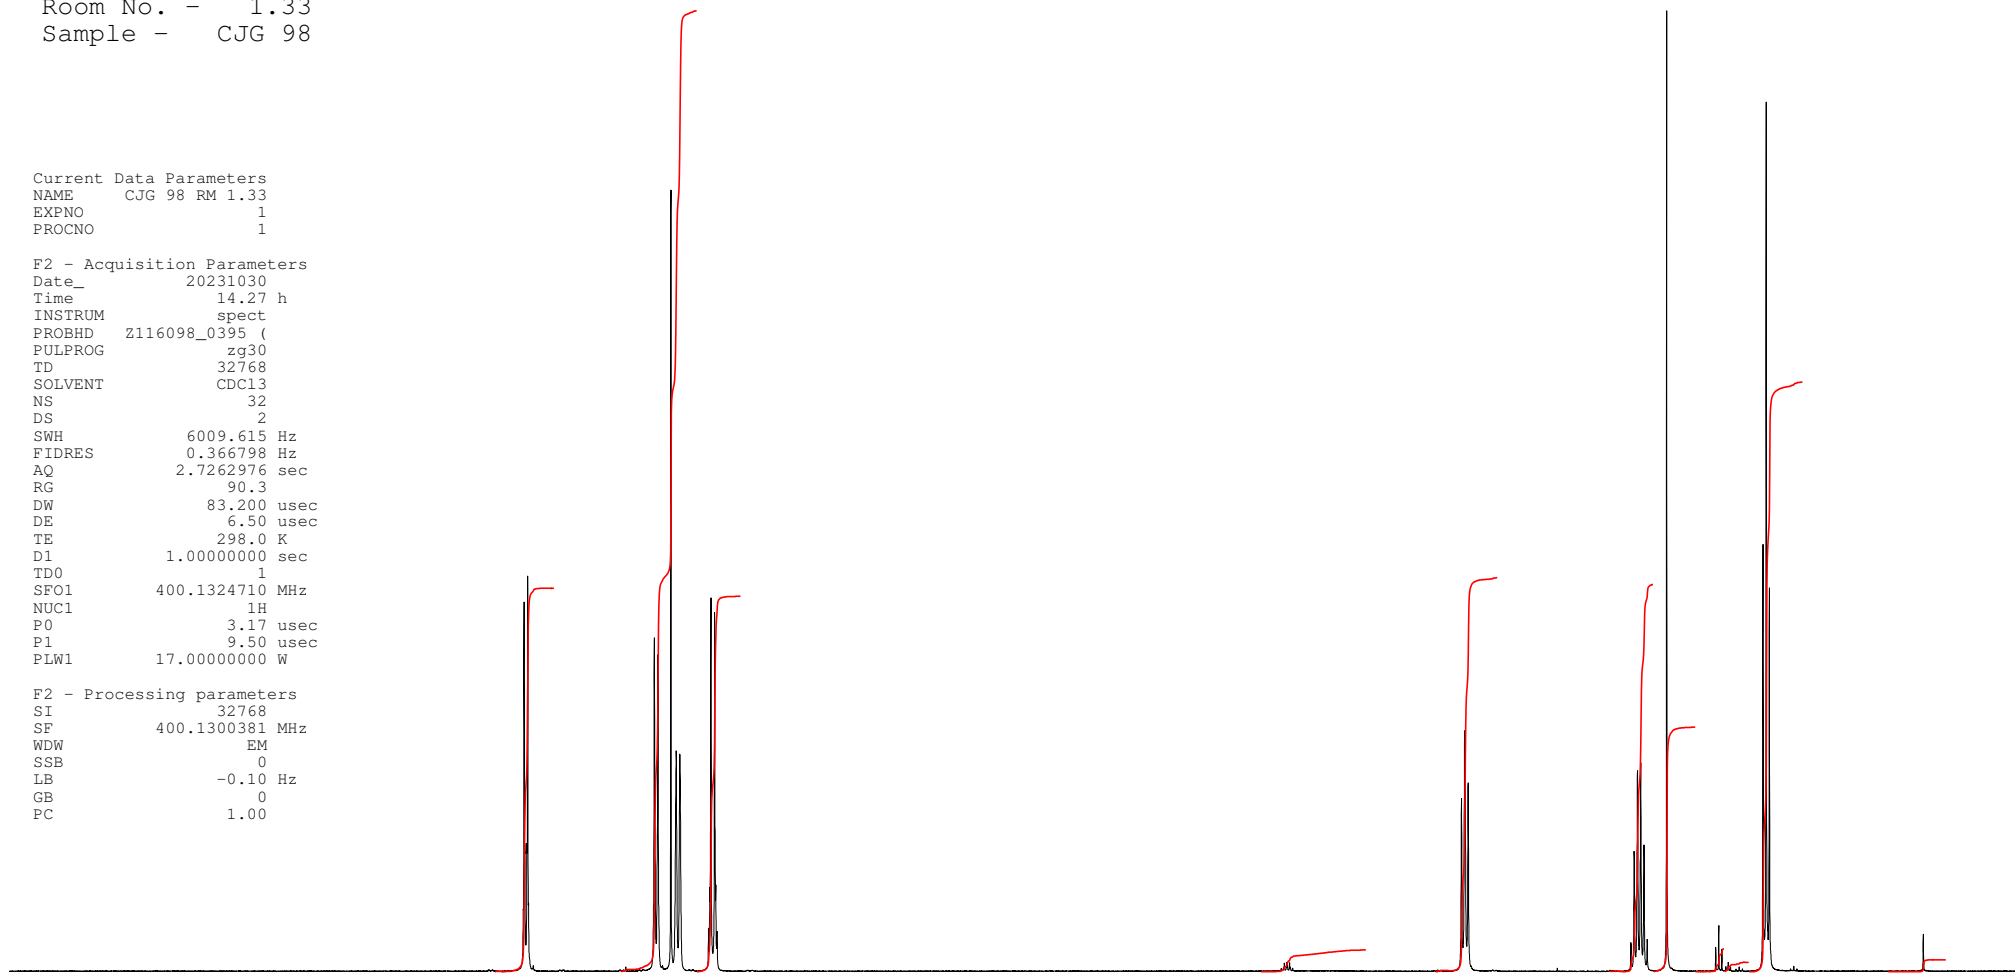

10

9

8

6

5

4

3

2

1

0

ppm

11.27

28.25

11.04

0.64

11.59

11.39

7.19

0.67

0.27

17.34

0.35