

8.06  
8.05  
8.04  
8.01  
7.99  
7.97  
7.58  
7.56  
7.56  
7.55  
7.54  
7.53  
7.53  
7.44  
7.41  
7.30  
7.30  
7.29  
7.28  
7.27  
7.27  
7.25  
7.23  
7.22  
7.20  
7.18

3.65  
3.63


2.64  
2.62  
2.60  
1.67  
1.65  
1.64  
1.62  
1.60  
1.58  
1.50  
1.18  
1.16  
1.15  
0.92  
0.90  
0.89  
0.88  
0.87  
-0.00

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 99

Current Data Parameters  
NAME CJG 99 RM 1.33  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20231031  
Time 10.50 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300415 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

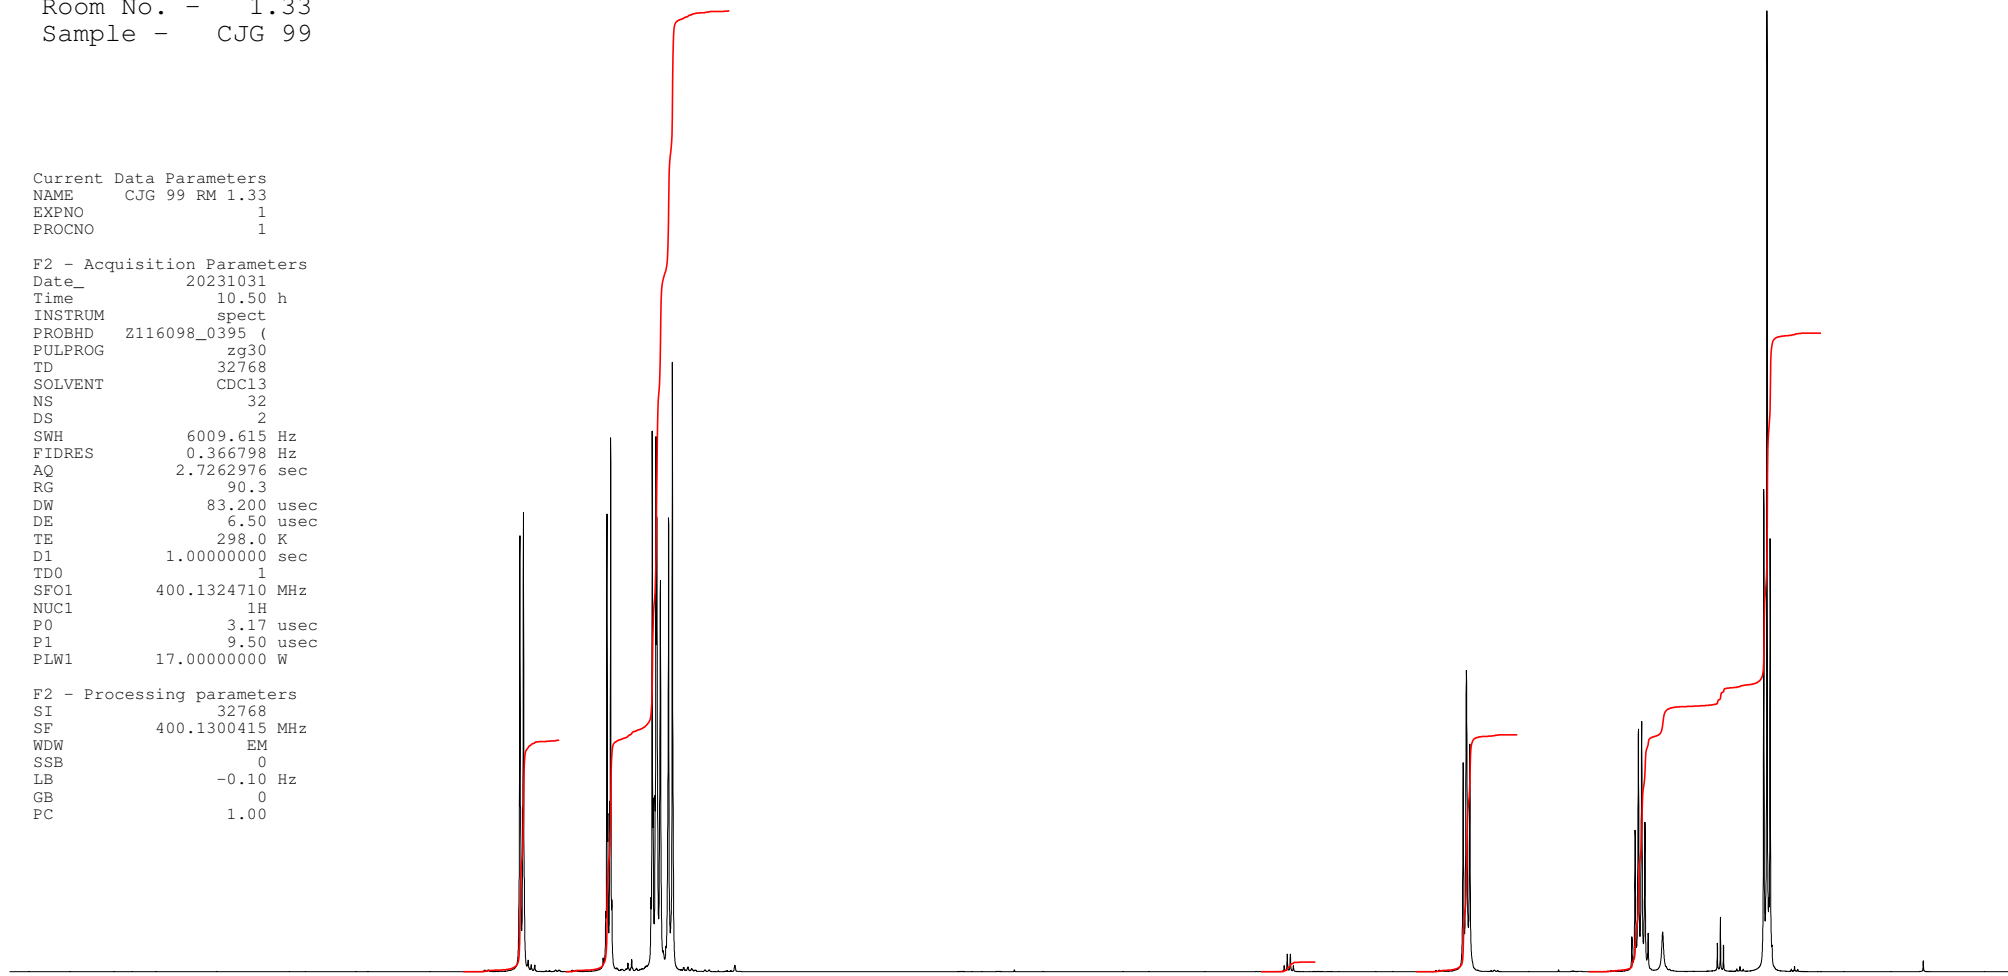

11.15  
46.24

0.47

11.40

30.74

0 ppm