

Name - Calum J Gibb  
Room No. - 1.33  
Sample - RM2931

Current Data Parameters  
NAME RM2931 RM 1.33  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20231115  
Time 12.20 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W


F2 - Processing parameters  
SI 32768  
SF 400.1300400 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.93  
7.91  
7.90  
7.66  
7.65  
7.63  
7.34  
7.33  
7.31  
7.29  
7.18  
7.05  
7.04  
7.03  
7.02  
6.99  
6.99  
6.97  
6.95  
6.93  
6.92

2.62  
2.61  
2.59

1.67  
1.65  
1.63  
1.61  
1.59  
1.58  
1.50  
0.92  
0.90  
0.88

-0.00

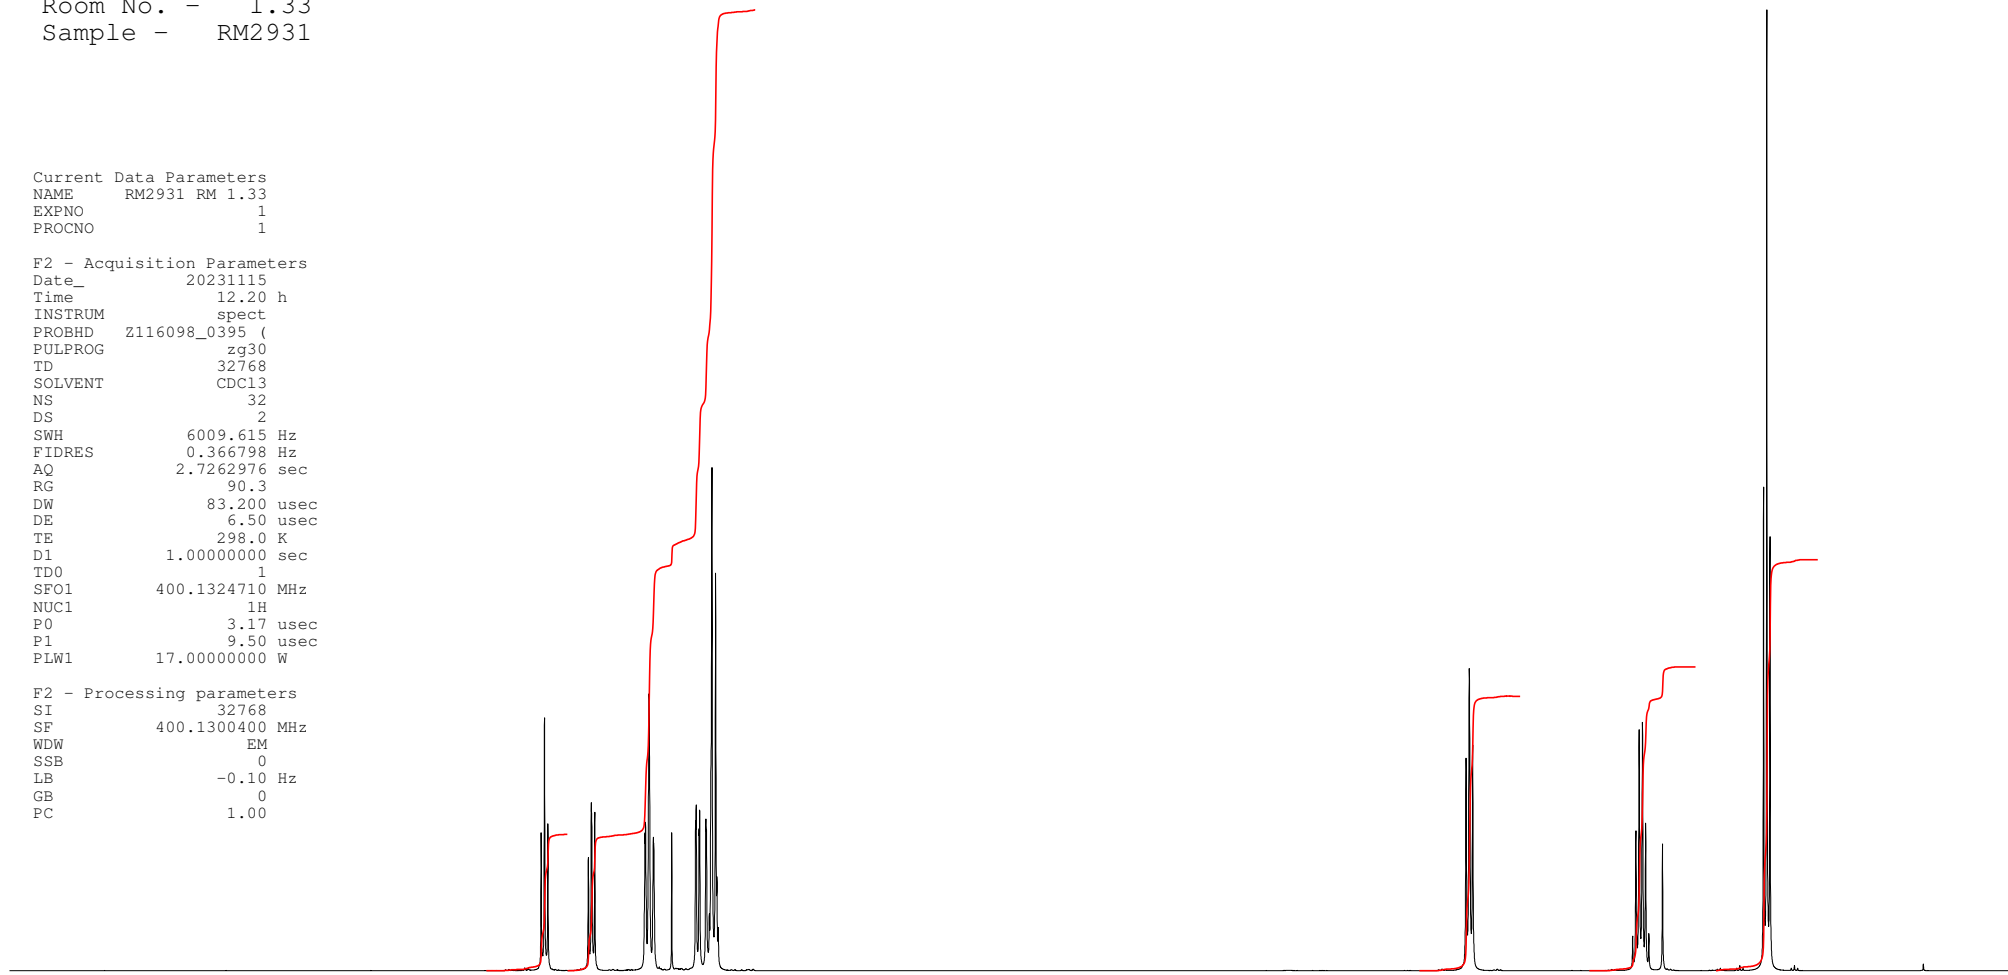

6.54  
46.05

13.16  
14.57  
19.69

0 ppm