

Name - Calum J Gibb  
 Room No. - 1.33  
 Sample - RM2933

Current Data Parameters  
 NAME RM2933 RM 1.33  
 EXPNO 1  
 PROCNO 1


F2 - Acquisition Parameters  
 Date\_ 20231114  
 Time 10.35 h  
 INSTRUM spect  
 PROBHD Z116098\_0395 (  
 PULPROG zg30  
 TD 32768  
 SOLVENT CDC13  
 NS 32  
 DS 2  
 SWH 6009.615 Hz  
 FIDRES 0.366798 Hz  
 AQ 2.7262976 sec  
 RG 90.3  
 DW 83.200 usec  
 DE 6.50 usec  
 TE 298.0 K  
 D1 1.00000000 sec  
 TD0 1  
 SFO1 400.1324710 MHz  
 NUC1 1H  
 P0 3.17 usec  
 P1 9.50 usec  
 PLW1 17.00000000 W

F2 - Processing parameters  
 SI 32768  
 SF 400.1300397 MHz  
 WDW EM  
 SSB 0  
 LB -0.10 Hz  
 GB 0  
 PC 1.00

7.97  
7.95  
7.93  
7.64  
7.62  
7.62  
7.60  
7.59  
7.58  
7.57  
7.56  
7.55  
7.55  
7.54  
7.42  
7.42  
7.40  
7.40  
7.37  
7.37  
7.34  
7.34  
7.31  
7.30  
7.29  
7.28  
7.28  
7.27  
7.19  
7.04  
7.04  
7.02  
7.02  
6.98  
6.98  
6.95  
6.95

2.62  
2.60  
2.58  
1.67  
1.65  
1.63  
1.61  
1.60  
1.58  
1.49  
1.18  
1.17  
1.15  
0.92  
0.90  
0.88

-0.00

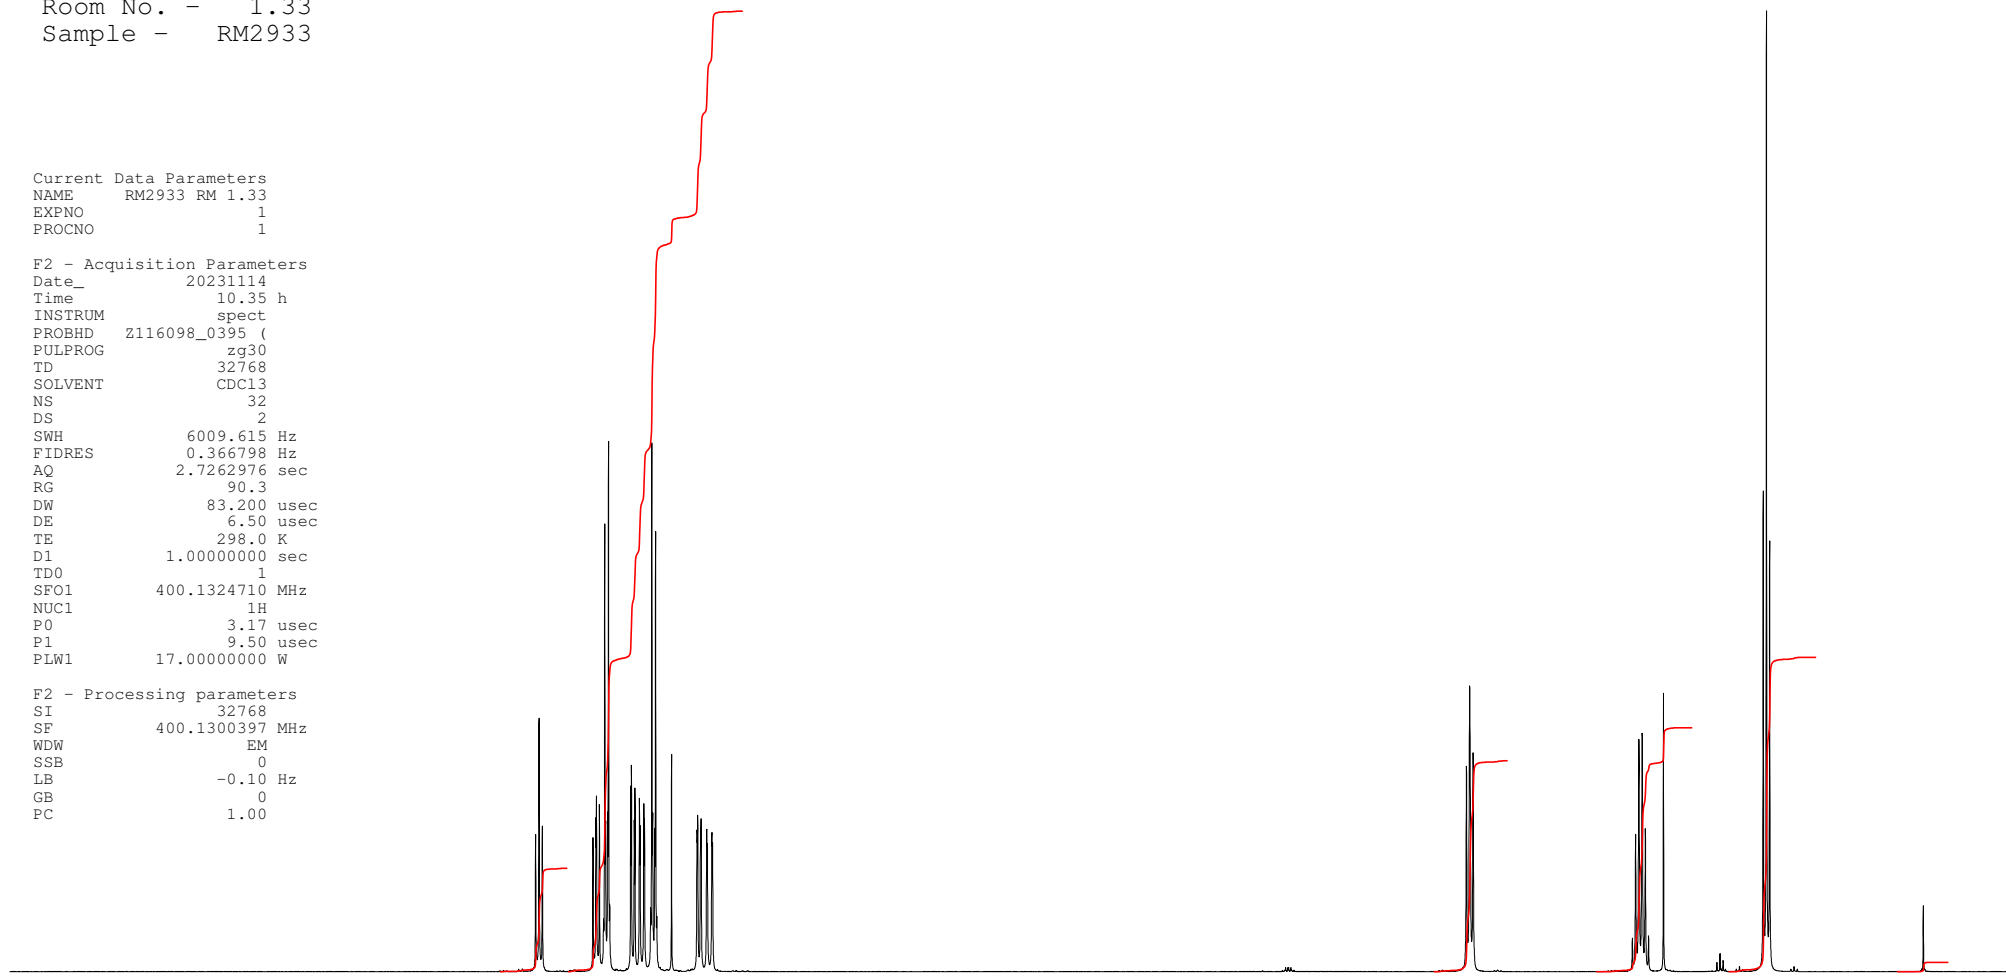

5.62  
52.13

11.44

13.24

17.05

0.52

0 ppm