

Name - Calum J Gibb  
Room No. - 1.33  
Sample - RM2934

Current Data Parameters  
NAME RM2934 RM 1.33  
EXPNO 1  
PROCNO 1


F2 - Acquisition Parameters  
Date\_ 20231114  
Time 10.25 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300400 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

7.97  
7.95  
7.93  
7.93  
7.67  
7.67  
7.66  
7.65  
7.62  
7.61  
7.60  
7.60  
7.59  
7.58  
7.57  
7.56  
7.55  
7.55  
7.29  
7.28  
7.28  
7.27  
7.26  
7.26  
7.18  
7.04  
7.03  
7.02  
7.01  
6.98  
6.98  
6.95  
6.95

2.62  
2.60  
2.58  
1.67  
1.65  
1.63  
1.61  
1.59  
1.58  
1.49  
1.18  
1.17  
1.15  
0.92  
0.90  
0.88

— 0.00

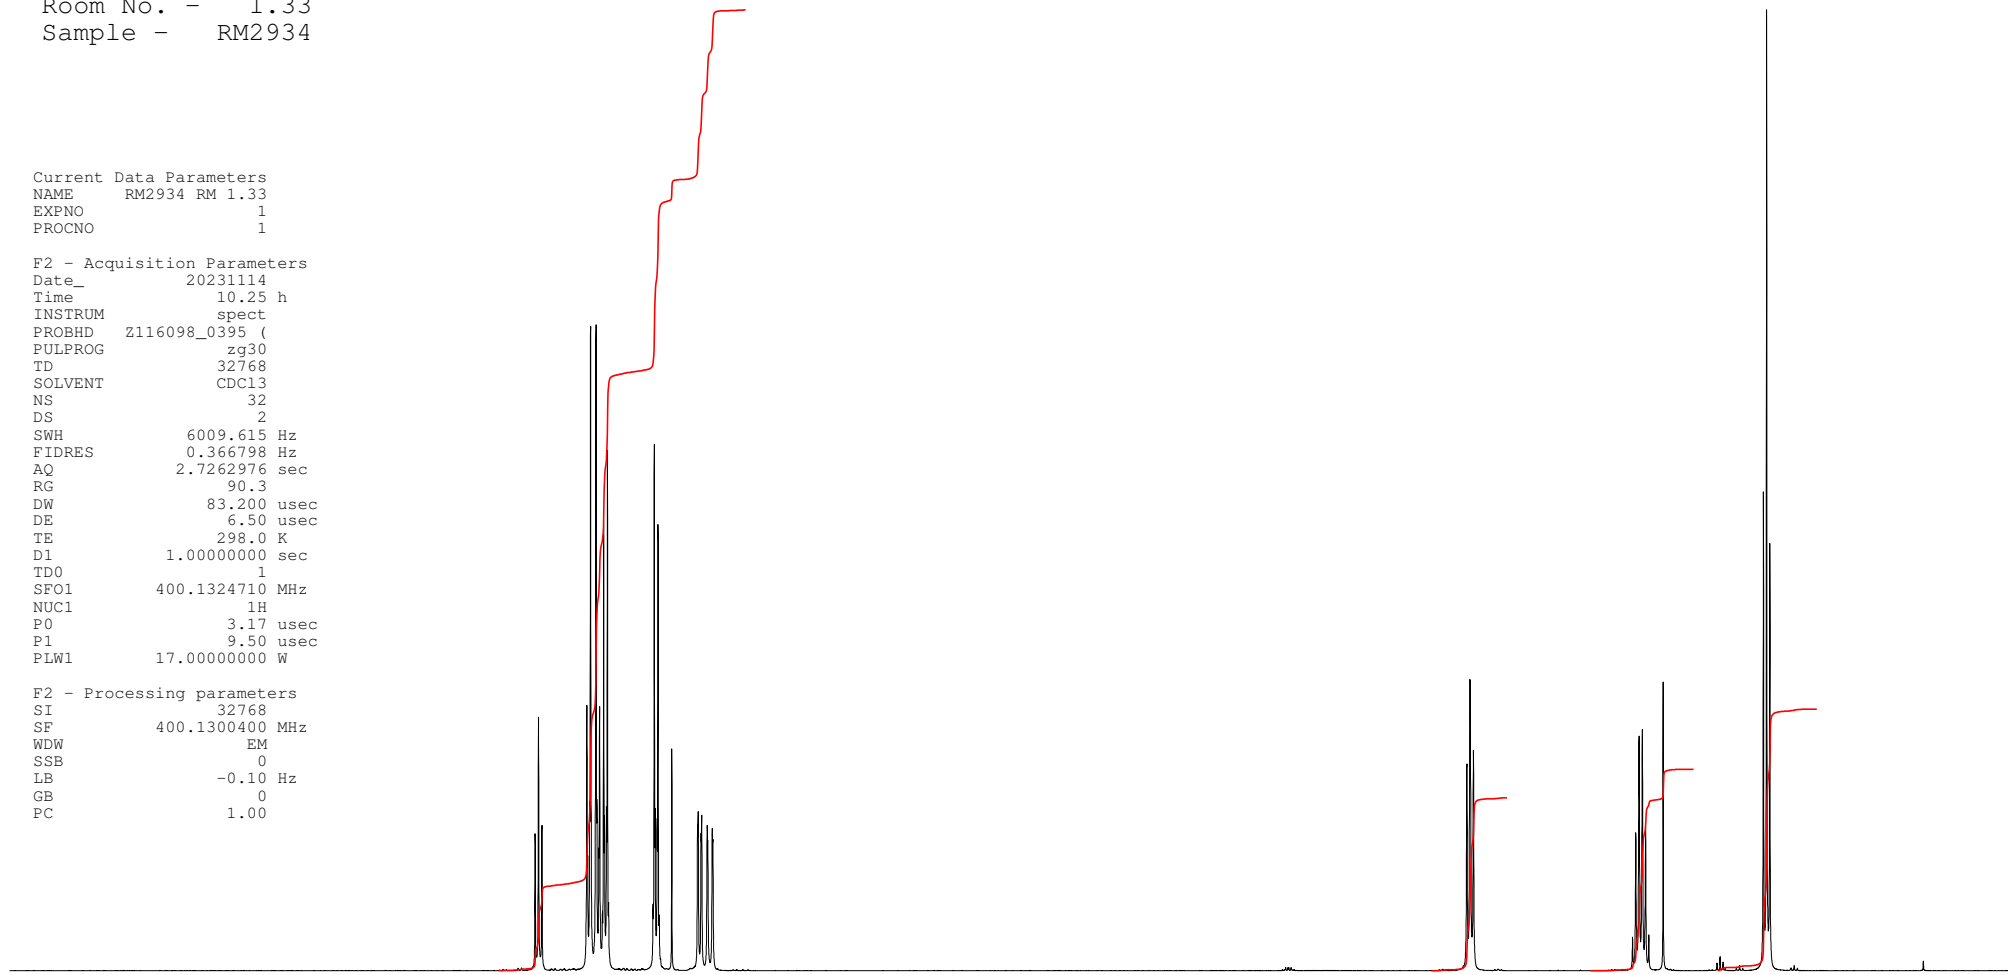

10

9

8

7

6

5

4

3

2

1

0 ppm

60.18

10.83

12.61

16.38