

Name - Calum J Gibb
 Room No. - 1.33
 Sample - CJG 199

Current Data Parameters
 NAME CJG 199 RM 1.33
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20240504
 Time 5.46 h
 INSTRUM spect
 PROBHD Z116098_0395 (
 PULPROG zg30
 TD 32768
 SOLVENT CDC13
 NS 32
 DS 2
 SWH 6009.615 Hz
 FIDRES 0.366798 Hz
 AQ 2.7262976 sec
 RG 90.3
 DW 83.200 usec
 DE 6.50 usec
 TE 298.0 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1324710 MHz
 NUC1 1H
 P0 3.17 usec
 P1 9.50 usec
 PLW1 17.00000000 W


F2 - Processing parameters
 SI 32768
 SF 400.1300392 MHz
 WDW EM
 SSB 0
 LB -0.10 Hz
 GB 0
 PC 1.00

7.94
7.92
7.90
7.70
7.68
7.53
7.51
7.19
7.05
7.03
6.99
6.98
6.97
6.96
6.94
6.93
6.93
6.92
6.81
6.79

2.63
2.60
2.58
2.56

1.66
1.64
1.62
1.60
1.58
1.57
1.49
0.92
0.90
0.88

-0.00

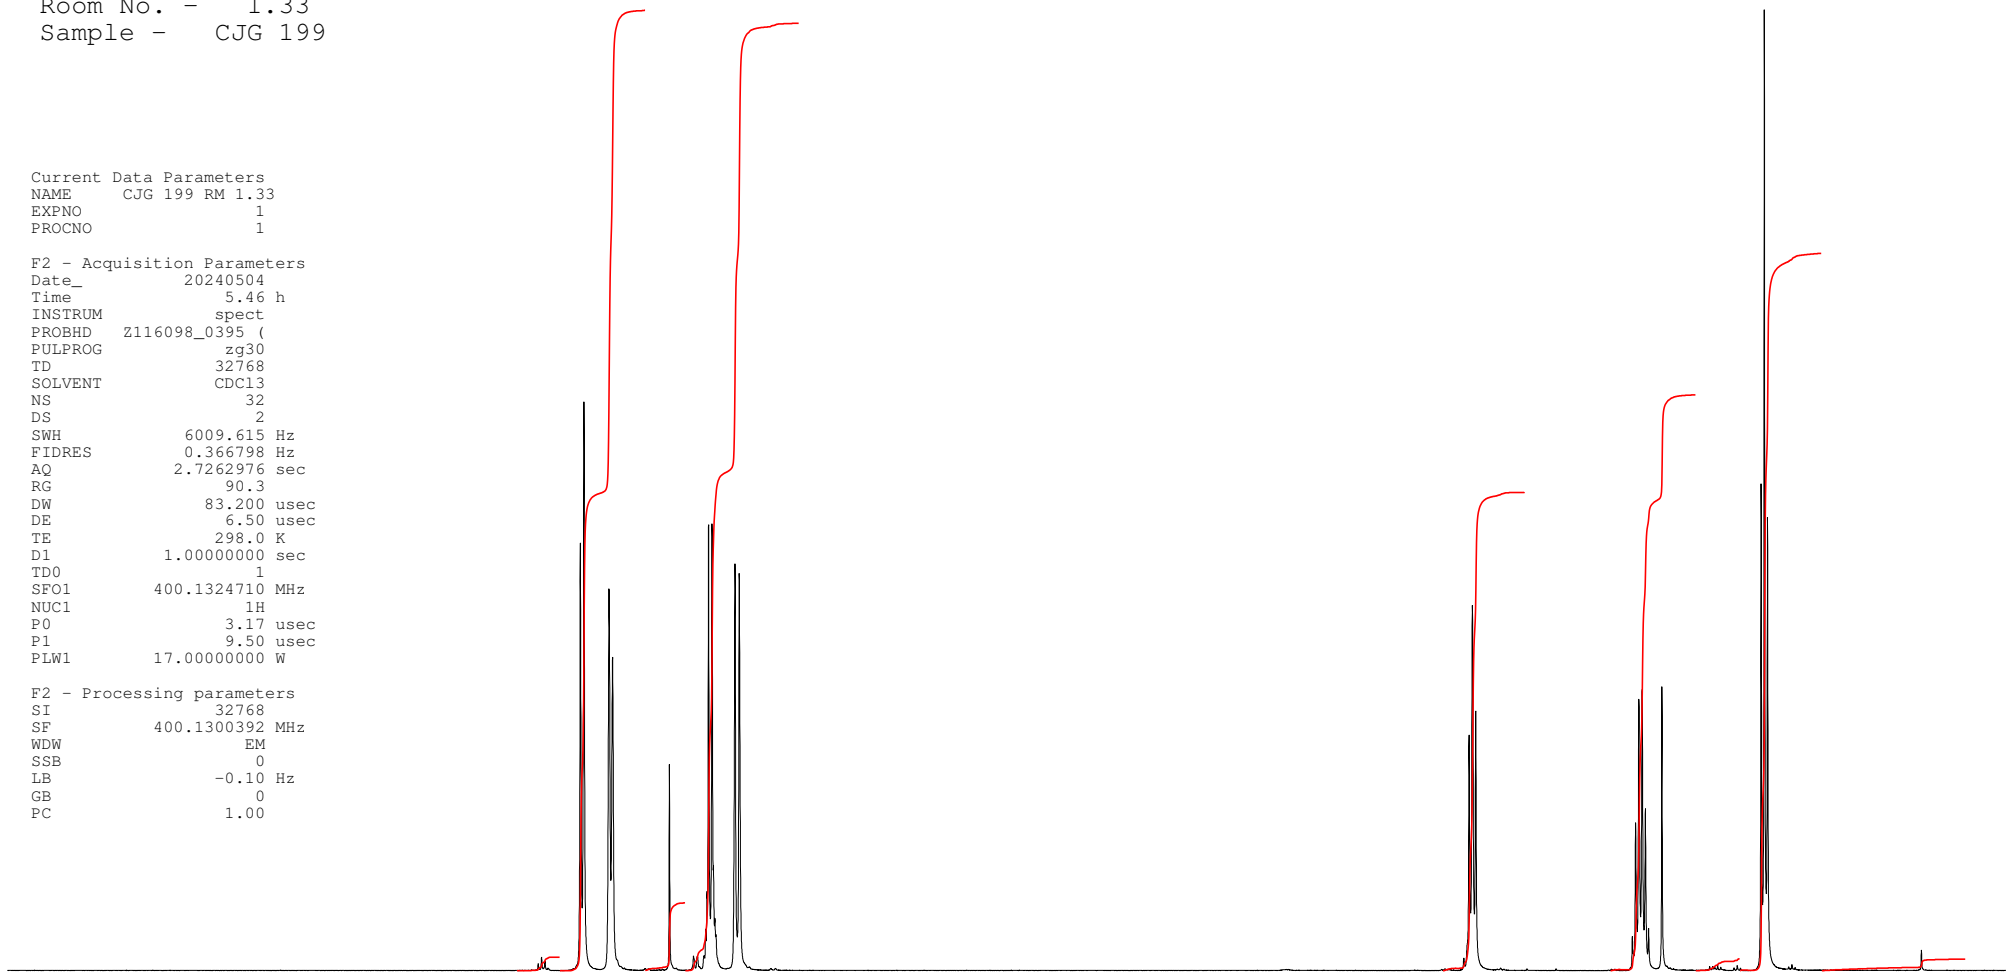

10

9

8

7

6

5

4

3

2

1

0

ppm