

Name - Calum J Gibb
Room No. - 1.33
Sample - CJG 272


Current Data Parameters
NAME CJG 272 (2) RM 1.33
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20241010
Time 11.50 h
INSTRUM spect
PROBHD Z116098_0395 (
PULPROG zg30
TD 32768
SOLVENT CDC13
NS 32
DS 2
SWH 6009.615 Hz
FIDRES 0.366798 Hz
AQ 2.7262976 sec
RG 90.3
DW 83.200 usec
DE 6.50 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324710 MHz
NUC1 1H
P0 3.17 usec
P1 9.50 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300000 MHz
WDW EM
SSB 0
LB -0.10 Hz
GB 0
PC 1.00

8.19
8.18
8.16
8.14
8.11
8.09
8.07
8.05
8.03
8.01
7.87
7.82
7.75
7.73
7.72
7.68
7.63
7.52
7.51
7.49
7.48
7.45
7.34
7.32
7.29
7.22
7.19
7.14
7.12
7.09
7.06
6.96
6.94

3.75
2.78
2.77
2.72
2.71
2.69
2.64
2.20
1.75
1.73
1.72
1.70
1.57
1.48
1.46
1.45
1.27
1.22
1.20
1.14
1.10
1.02
1.00
0.98
0.91
0.90
0.86
0.84

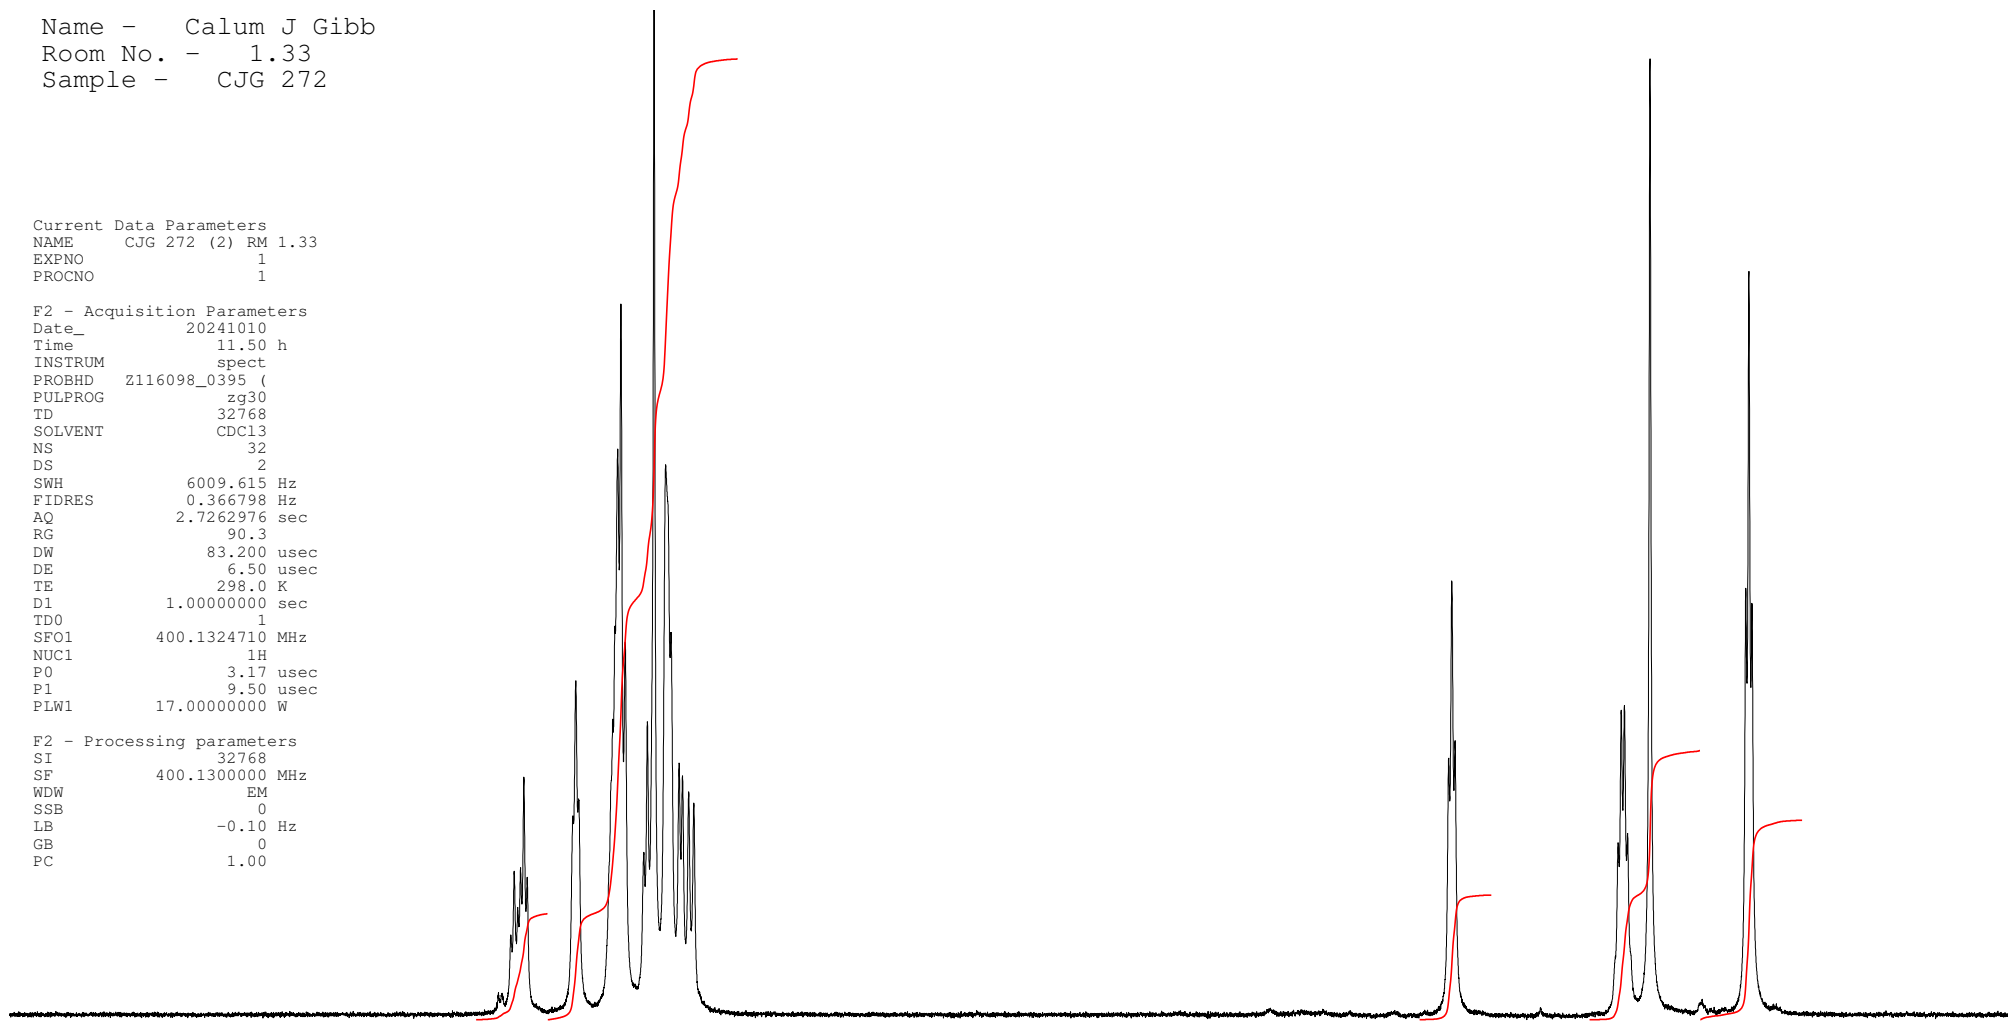

6.39
57.87

7.50

16.22

12.02

0 ppm