

Name - Calum J Gibb
 Room No. - 1.33
 Sample - CJG 110


Current Data Parameters
 NAME CJG 110 (2) RM 1.33
 EXPNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20241011
 Time 12.36 h
 INSTRUM spect
 PROBHD Z116098_0395 (
 PULPROG zg30
 TD 32768
 SOLVENT CDC13
 NS 32
 DS 2
 SWH 6009.615 Hz
 FIDRES 0.366798 Hz
 AQ 2.7262976 sec
 RG 79.8
 DW 83.200 usec
 DE 6.50 usec
 TE 298.0 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1324710 MHz
 NUC1 1H
 P0 3.17 usec
 P1 9.50 usec
 PLW1 17.00000000 W

F2 - Processing parameters
 SI 32768
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB -0.10 Hz
 GB 0
 PC 1.00

8.03
7.78
7.78
7.76
7.76
7.69
7.69
7.67
7.54
7.53
7.52
7.52
7.51
7.49
7.28
7.23
7.23
7.22
7.21
7.21
7.19
7.18
7.17
7.16
7.14
7.12
7.08
7.05
6.90
6.88

2.72
2.69
2.67
2.65
1.75
1.75
1.74
1.72
1.70
1.68
1.66
1.60
1.36
1.26
1.02
1.00
0.98

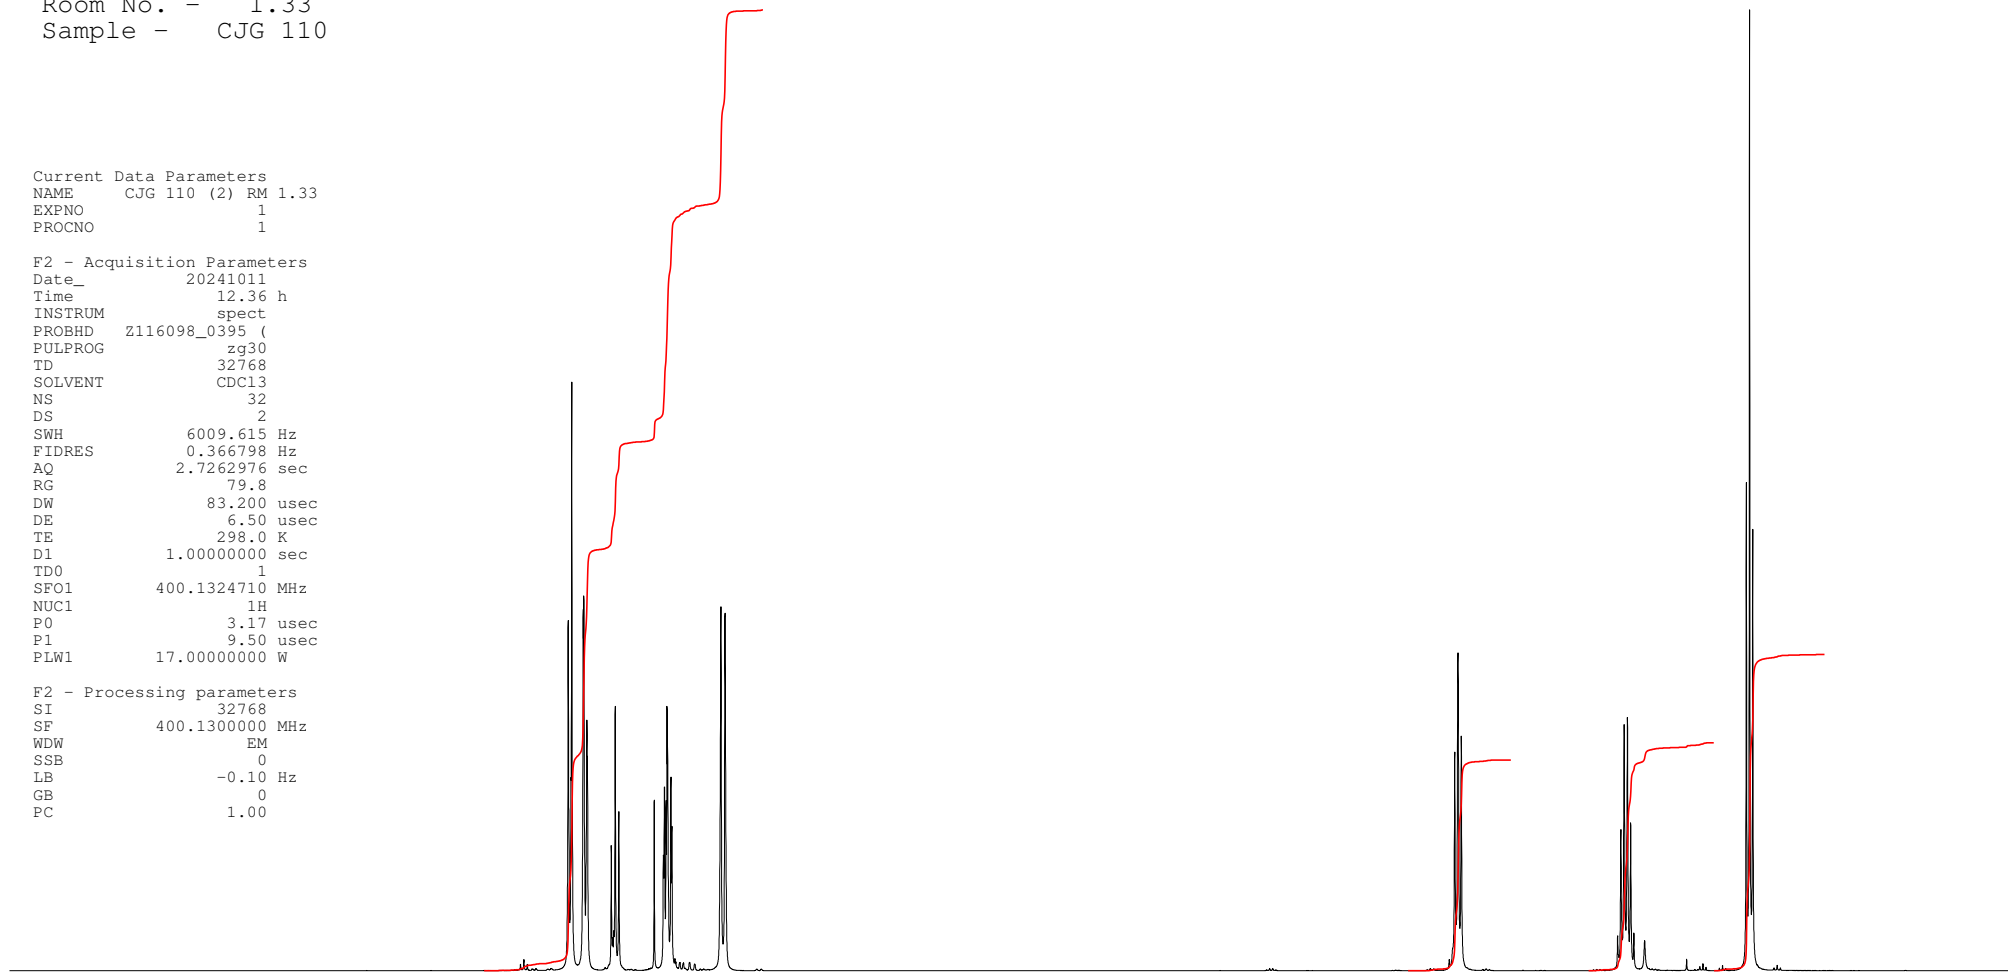

56.00

12.28

13.29

18.43

0 ppm