

8.15  
8.13  
7.75  
7.73  
7.71  
7.55  
7.53  
7.52  
7.51  
7.50  
7.49  
7.49  
7.48  
7.47  
7.45  
7.37  
7.35  
7.28  
7.21  
7.20  
7.20  
7.19  
7.19  
7.17  
7.16


2.74  
2.73  
2.71  
1.77  
1.76  
1.74  
1.72  
1.70  
1.68  
1.58  
1.29  
1.27  
1.25  
1.02  
1.00  
0.98

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 213

Current Data Parameters  
NAME CJG 213 RM 1.33  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240516  
Time 12.18 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

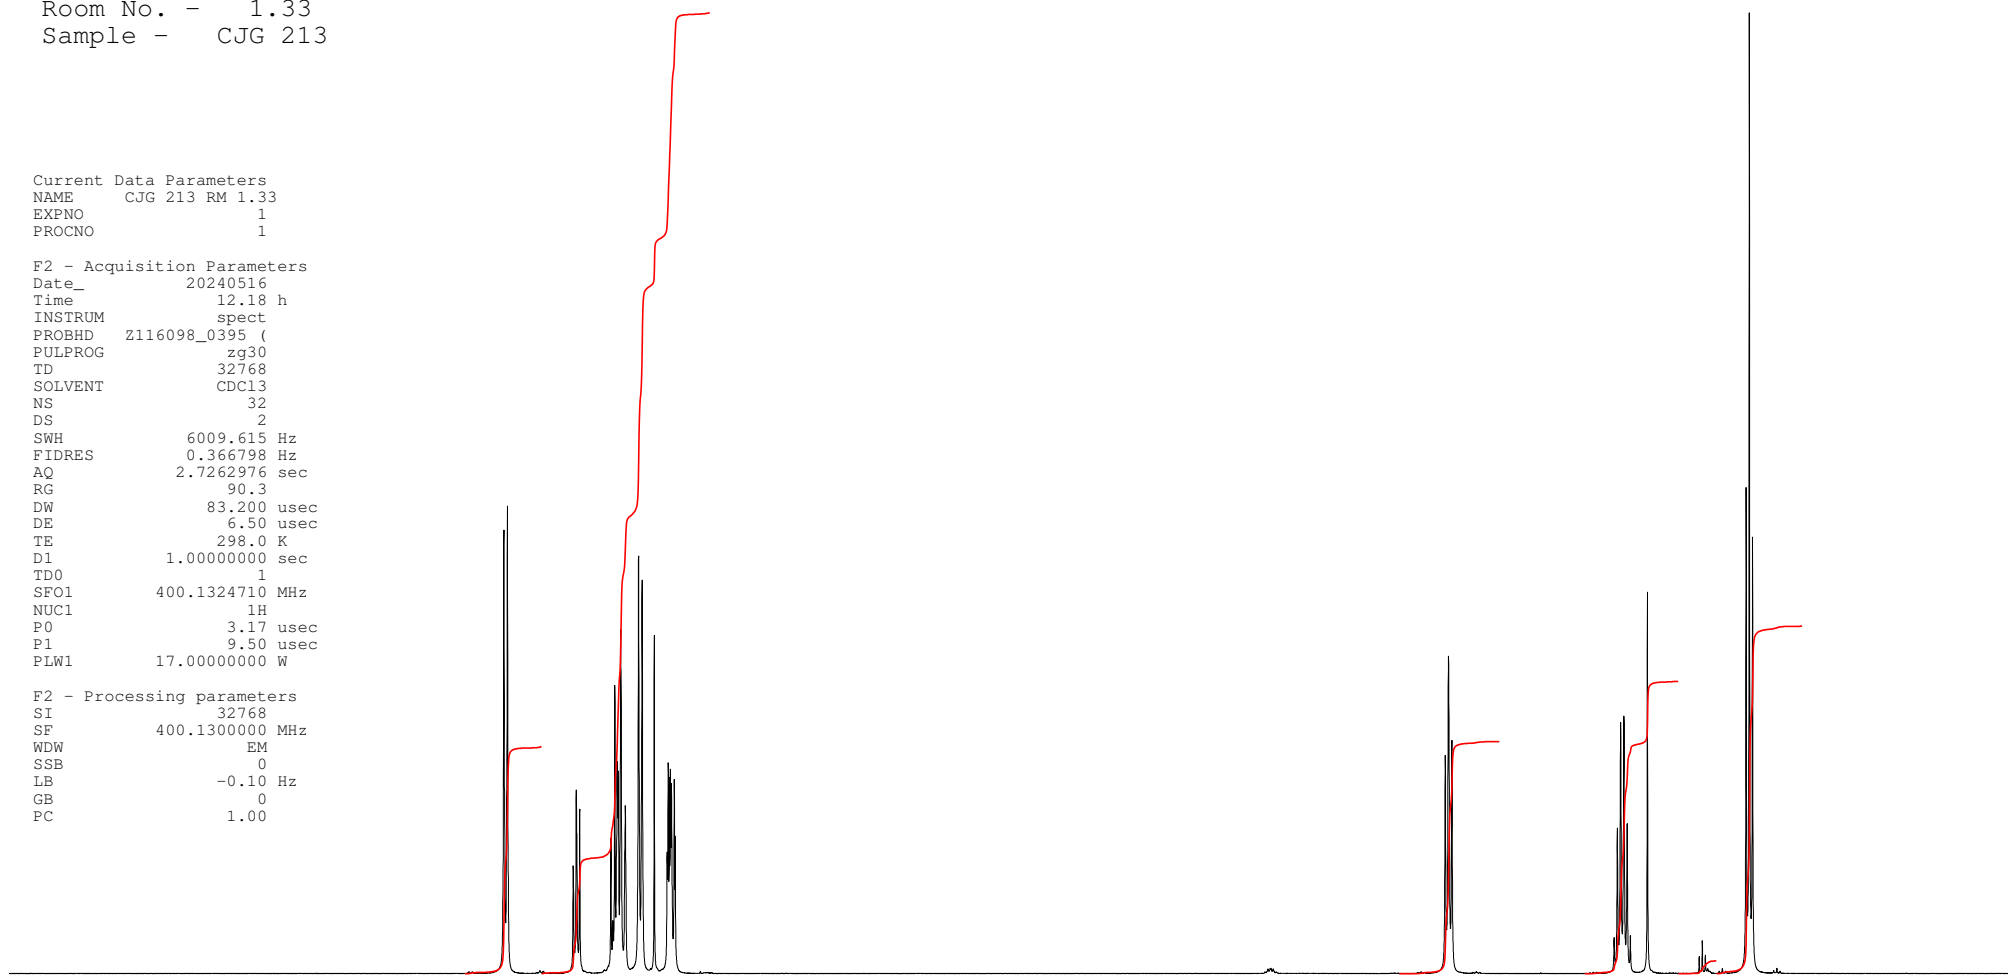

10.96  
46.35

11.19  
14.11  
0.62  
16.77

0 ppm