

7.93  
7.91  
7.89  
7.67  
7.65  
7.65  
7.63  
7.34  
7.34  
7.32  
7.29  
7.29  
7.19  
7.05  
7.05  
7.03  
7.03  
6.99  
6.99  
6.97  
6.96  
6.96  
6.94  
6.93  
6.92


2.65  
2.63  
2.61  
2.10  
1.97  
1.61  
1.59  
1.59  
1.58  
1.57  
1.57  
1.55  
1.54  
1.49  
1.36  
1.34  
1.32  
1.30  
1.28  
1.26  
1.19  
1.19  
1.17  
1.15  
1.14  
0.90  
0.88

Name - Calum J Gibb  
Room No. - 1.33  
Sample - CJG 103

Current Data Parameters  
NAME CJG 103 RM 1.33  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20231121  
Time 16.32 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300389 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

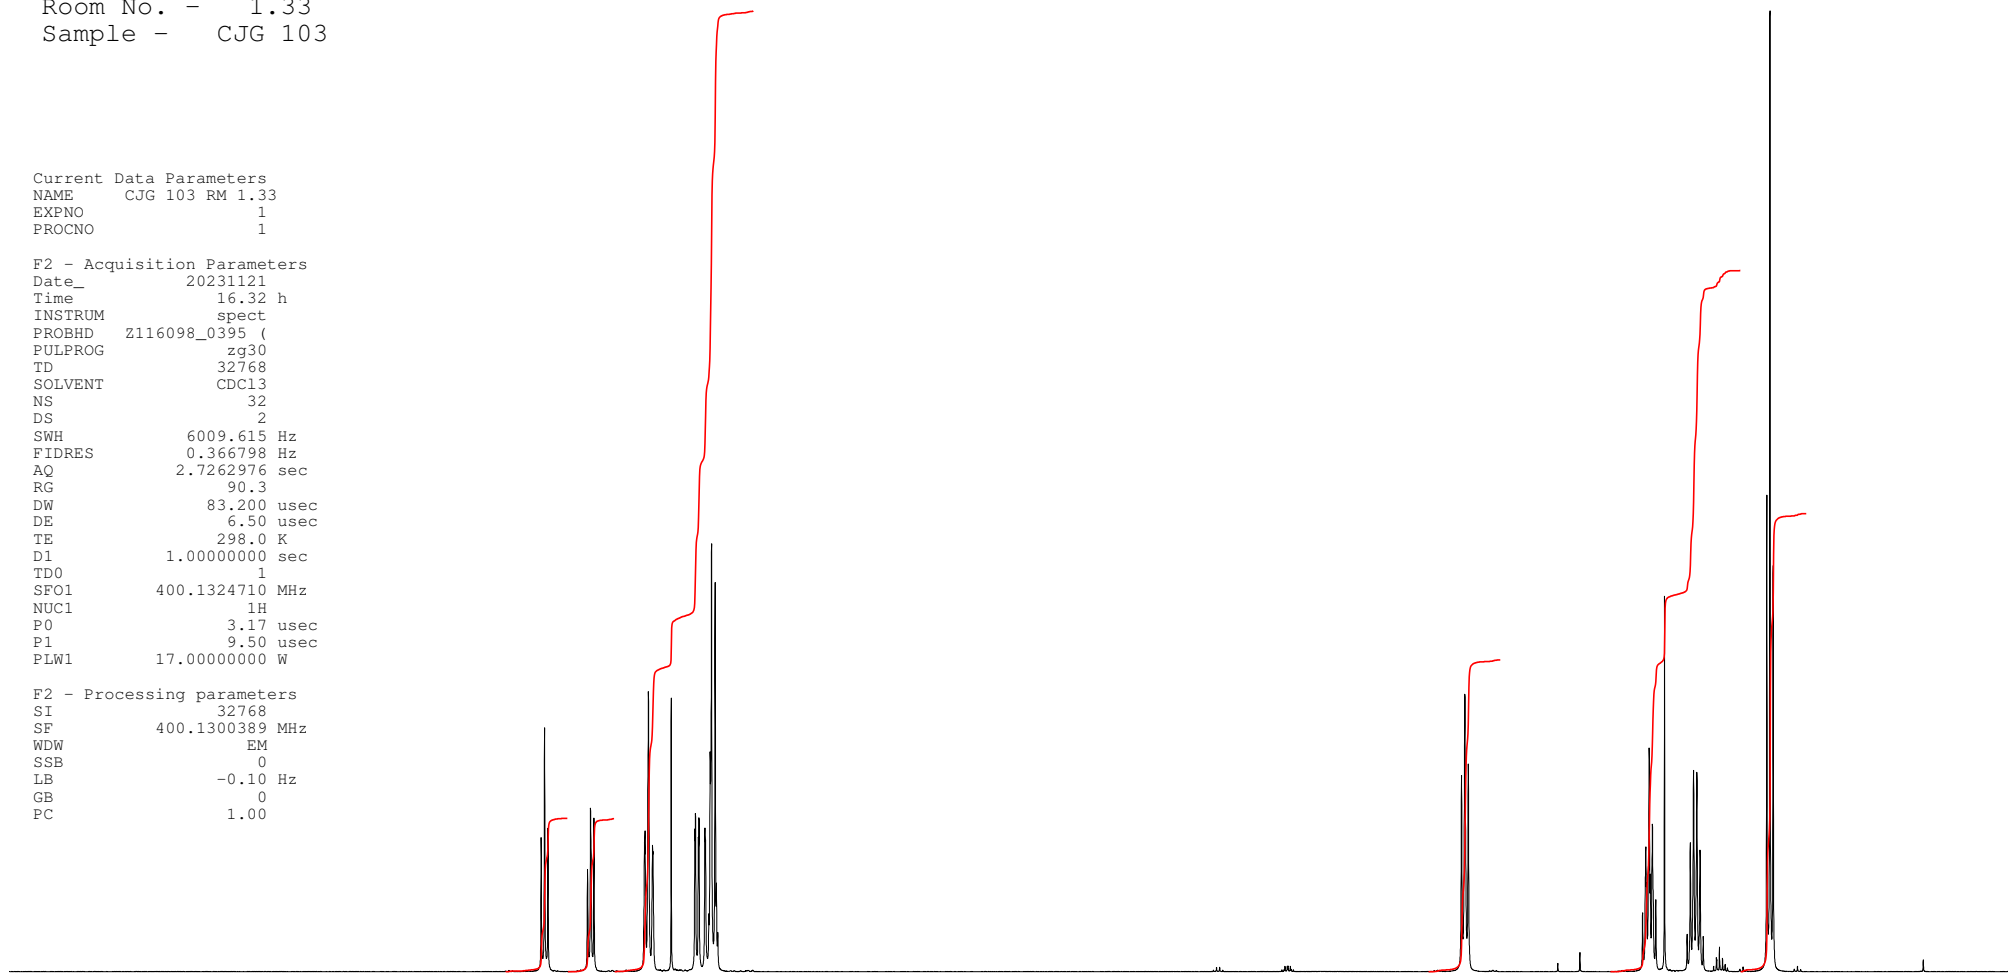

5.60  
5.60  
35.08

11.38  
25.61  
16.73

0 ppm