

7.62  
7.60  
7.58  
7.57  
7.56  
7.55  
7.54  
7.54  
7.20  
7.18  
7.18  
7.14  
7.13  
7.12  
7.11  
7.11  
7.10  
6.96  
6.94  
6.93  
6.92  
6.91  
6.89


2.55  
2.53  
2.51  
1.74  
1.72  
1.70  
1.68  
1.66  
1.47  
1.45  
1.43  
1.41  
1.39  
1.37  
1.36  
1.14  
1.13  
0.94  
0.92  
0.90

Name - sTUART berrow  
Group initials - RJM  
Room No. - Bragg 1.12  
Sample - SRB-CHEM-093

Current Data Parameters  
NAME 25.10.02-SRB-CHEM-093  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20251002  
Time 16.04 h  
INSTRUM spect  
PROBHD Z116098\_0395 (  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 32  
DS 2  
SWH 6009.615 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 90.3  
DW 83.200 usec  
DE 6.50 usec  
TE 298.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324710 MHz  
NUC1 1H  
P0 3.17 usec  
P1 9.50 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.1300399 MHz  
WDW EM  
SSB 0  
LB -0.10 Hz  
GB 0  
PC 1.00

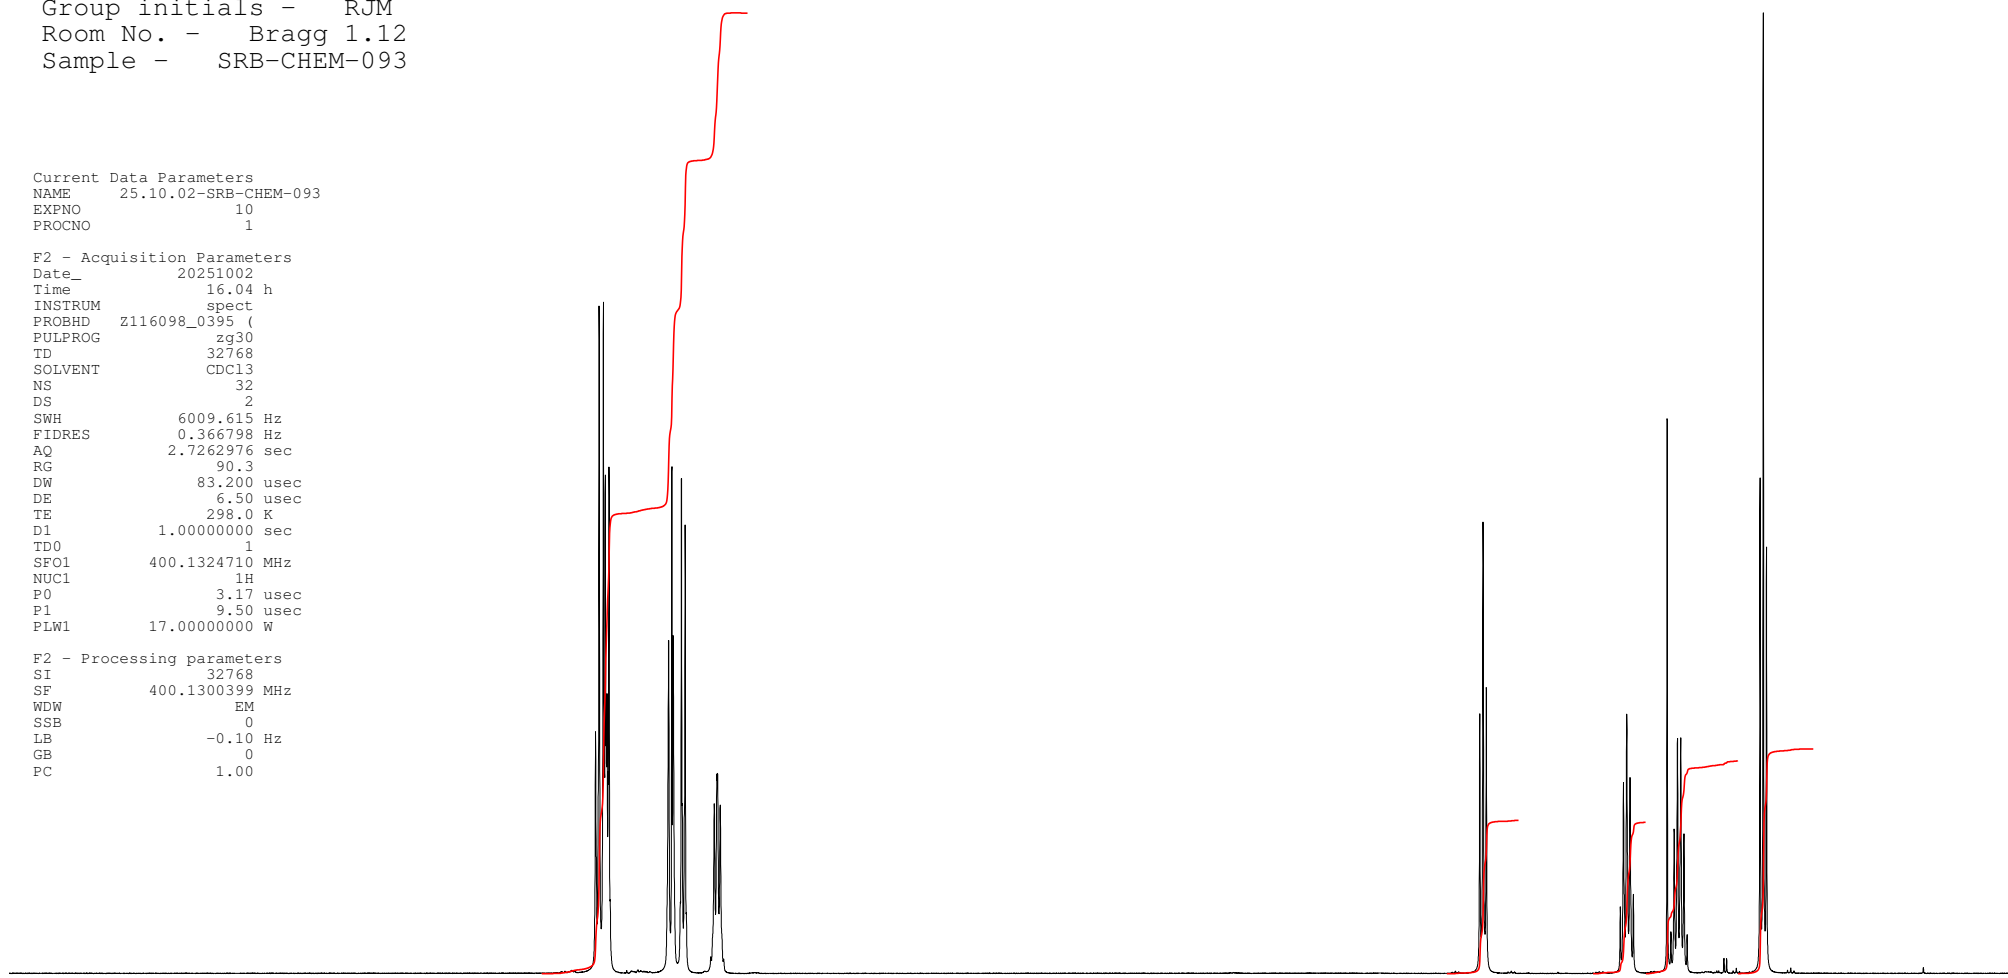

56.40

9.00

8.89

12.51

13.20

0 ppm